

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101517\
 Data File : BG029241.D
 Acq On : 15 Oct 2017 2:54
 Operator : SJ/JU
 Sample : I5548-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Oct 15 04:17:08 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Oct 15 01:38:25 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	109766	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	500795	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.79	164	299828	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.52	188	646246	20.00	ng/ul	0.00
75) Chrysene-d12	21.80	240	585912	20.00	ng/ul	0.00
83) Perylene-d12	25.11	264	586845	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.55	96	10524	3.90	ng/uL	0.00
5) Phenol-d5	7.32	99	212634	20.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.49	67	133725	20.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.70	132	151745	20.42	ng/ul	0.00
13) 4-Methylphenol-d8	8.87	113	154036	18.10	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	79740	22.18	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	87192	23.67	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	163982	19.54	ng/ul	0.00
29) 4-Chloroaniline-d4	11.11	131	153854	15.78	ng/ul	0.00
43) Dimethylphthalate-d6	14.19	166	525325	20.49	ng/ul	0.00
46) Acenaphthylene-d8	14.49	160	649961	20.85	ng/ul	0.00
51) 4-Nitrophenol-d4	14.97	143	79765	16.86	ng/ul	0.00
57) Fluorene-d10	15.78	176	446378	21.26	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.89	200	52556	16.66	ng/ul	0.00
70) Anthracene-d10	17.62	188	624077	20.42	ng/ul	0.00
76) Pyrene-d10	19.90	212	640740	21.13	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.88	264	547311	19.69	ng/ul	0.00

Target Compounds


						Ovalue
6) Phenol	7.35	94	21841	2.00	ng/ul	94
44) Dimethylphthalate	14.23	163	230957	9.24	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101517\
Data File : BG029241.D
Acq On : 15 Oct 2017 2:54
Operator : SJ/JU
Sample : I5548-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Oct 15 04:17:08 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Oct 15 01:38:25 2017
Response via : Initial Calibration

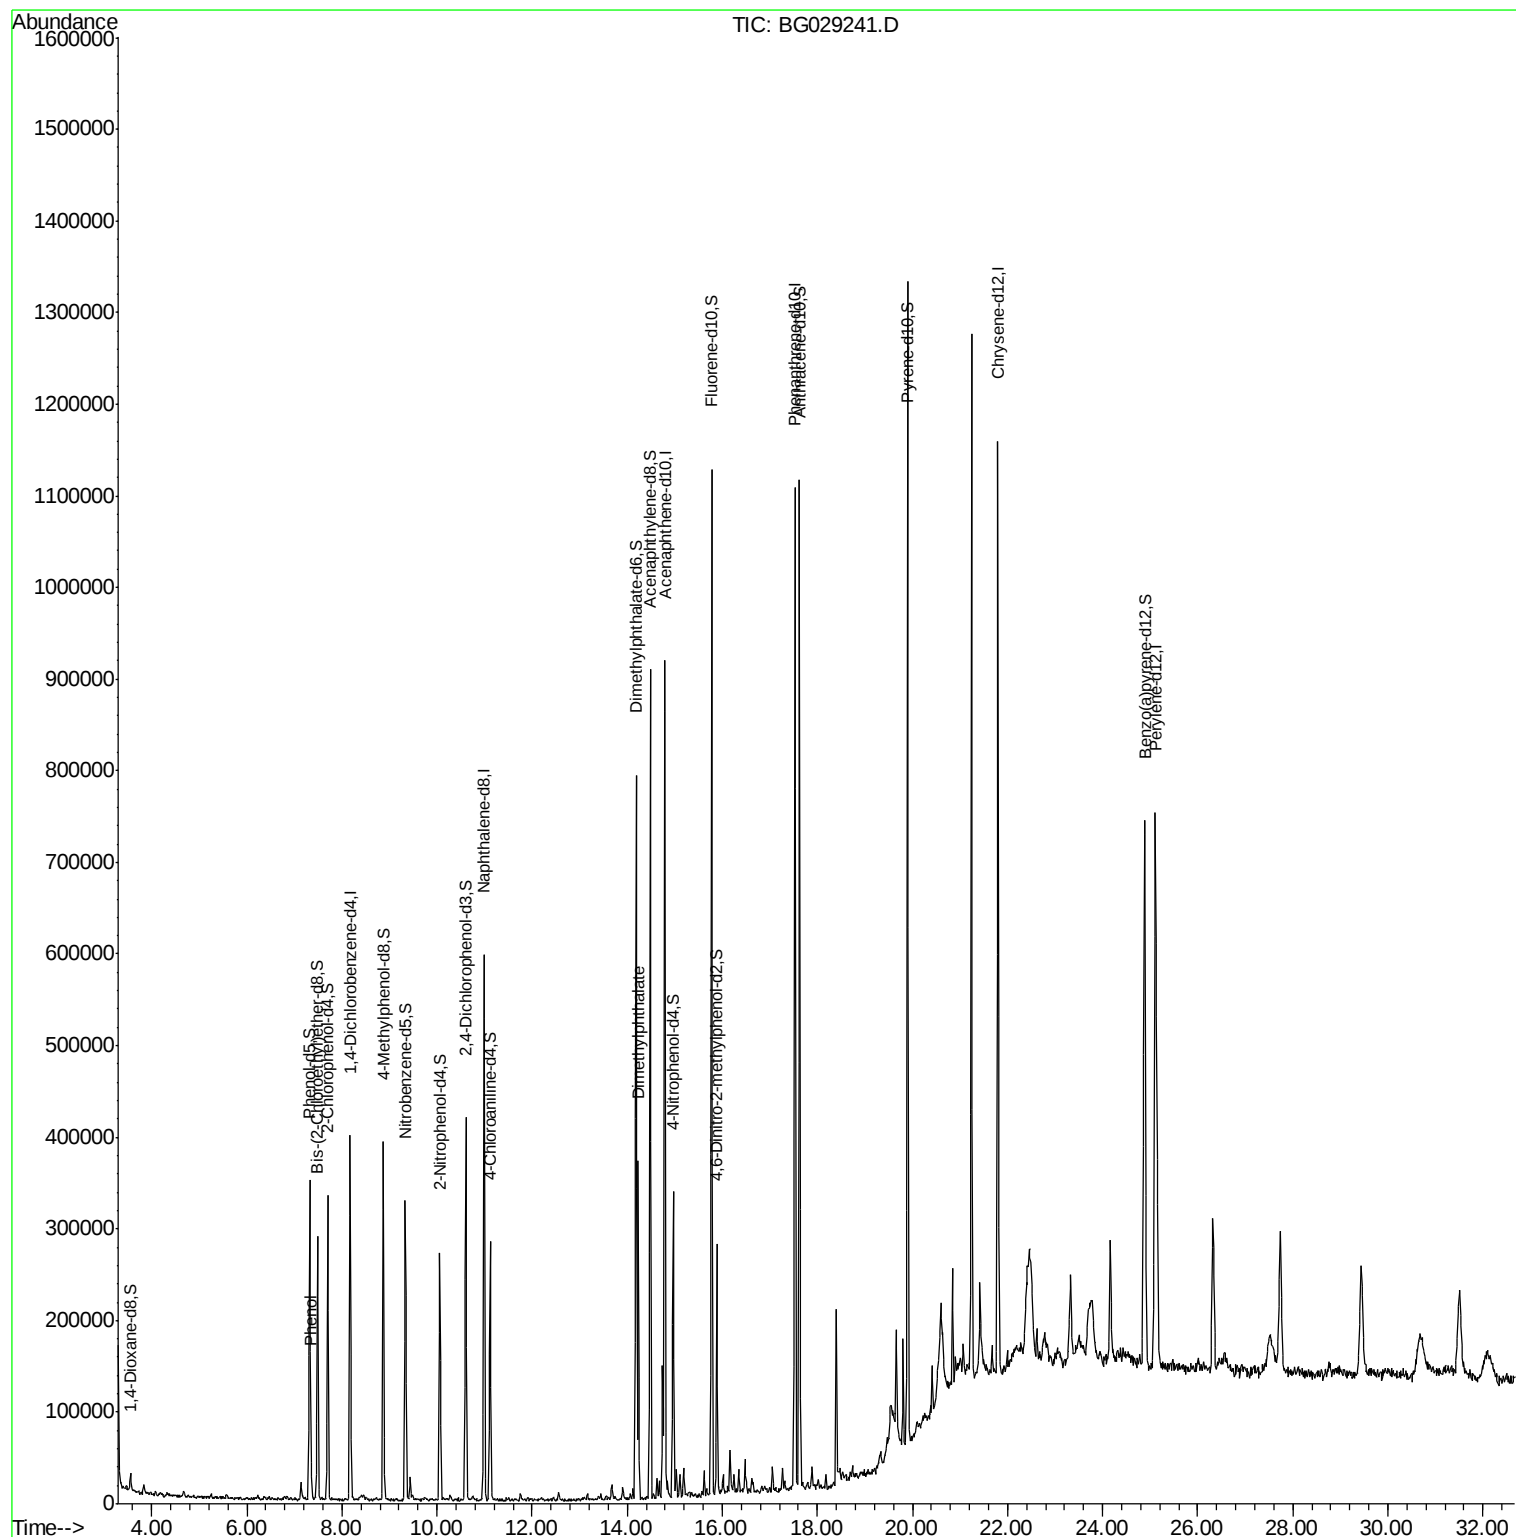

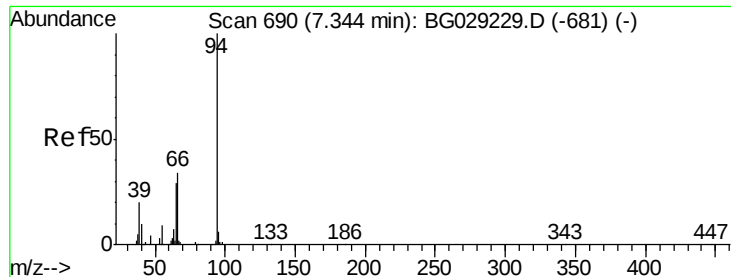

#6

Phenol

Concen: 2.00 ng/ul

RT: 7.35 min Scan# 691

Delta R.T. 0.00 min

Lab File: BG029241.D

Acq: 15 Oct 2017 2:54

Instrument :

BNA_G

ClientSampleId :





Tot Ion: 94 Resp: 21841

Ion Ratio Lower Upper

94 100

65 36.0 27.1 40.7

66 48.7 34.6 52.0

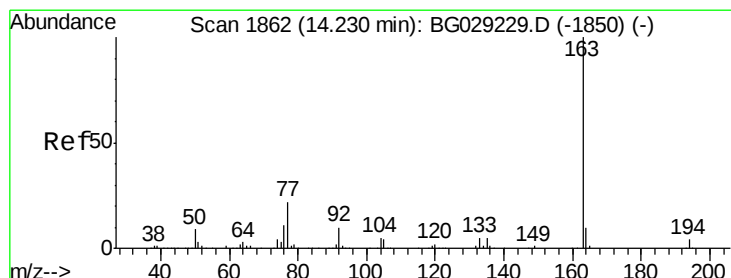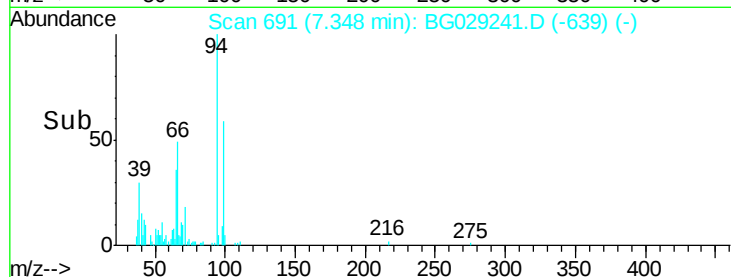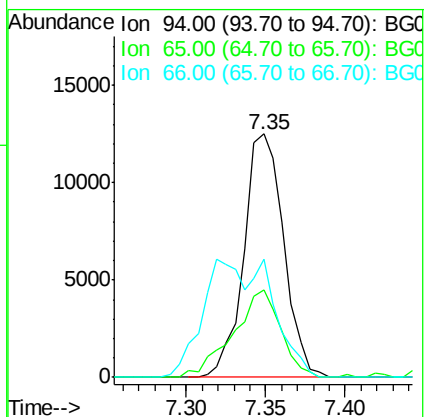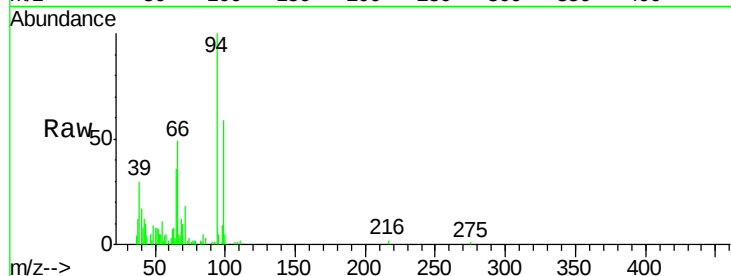

#44

Dimethylphthalate

Concen: 9.24 ng/ul

RT: 14.23 min Scan# 1863

Delta R.T. 0.00 min

Lab File: BG029241.D

Acq: 15 Oct 2017 2:54

Tgt Ion: 163 Resp: 230957

Ion Ratio Lower Upper

163 100

194 4.6 3.5 5.3

164 9.4 7.6 11.4

