
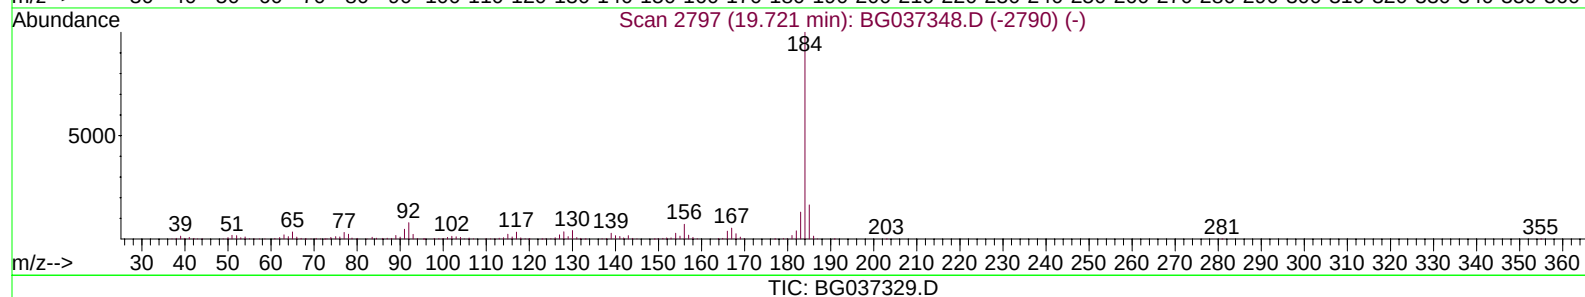
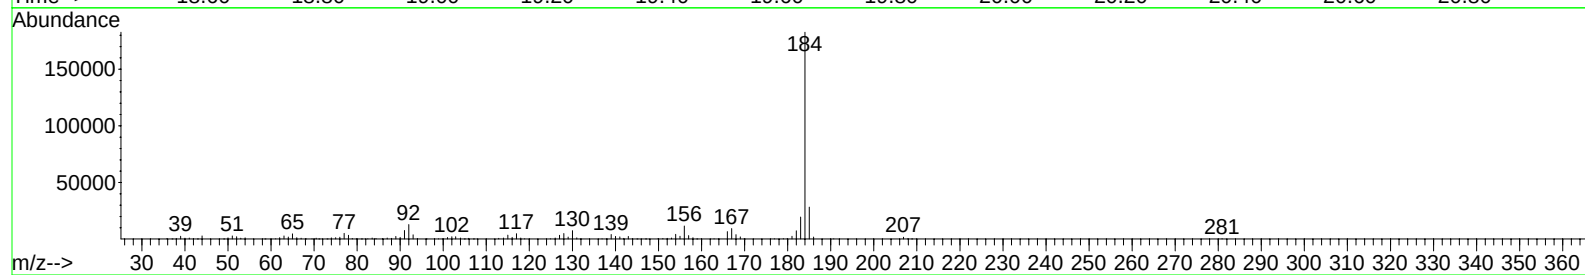


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101518\
Data File : BG037329.D
Acq On : 15 Oct 2018 11:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 07:00:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

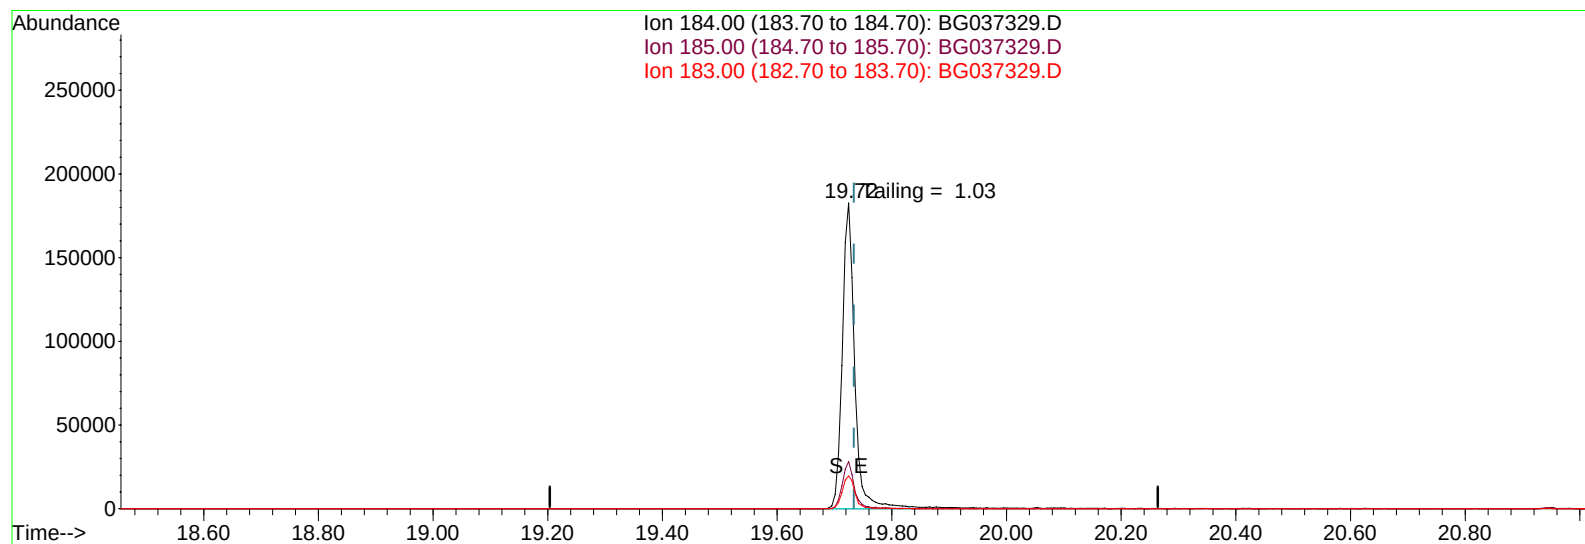

(77) Benzidine




19.725min (-0.009) 0.00ng

response 273074

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.45
183.00	12.70	10.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101518\
Data File : BG037329.D
Acq On : 15 Oct 2018 11:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 07:00:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

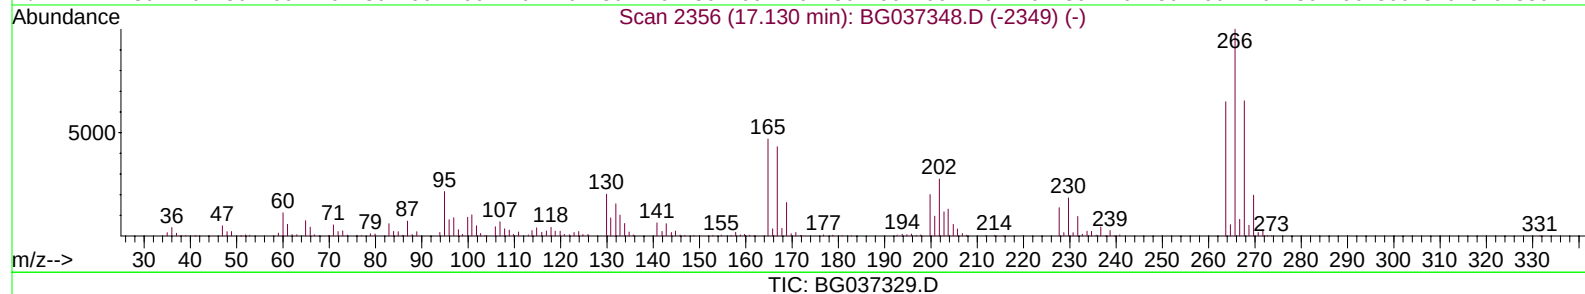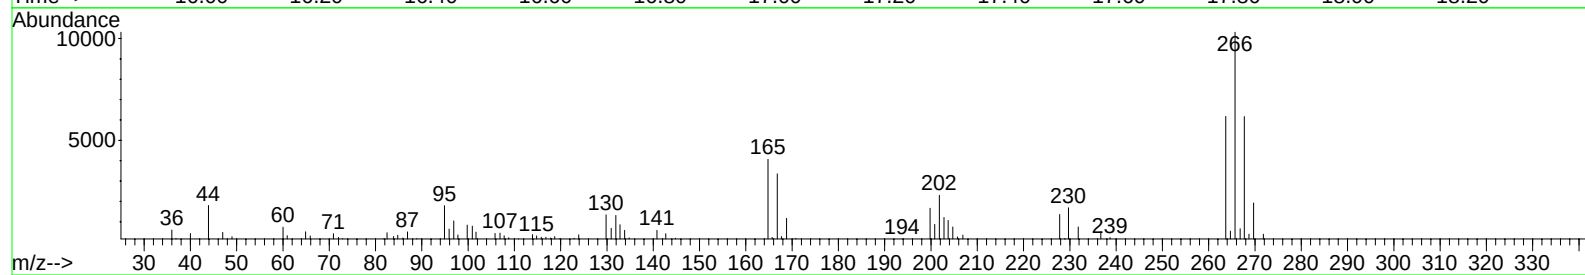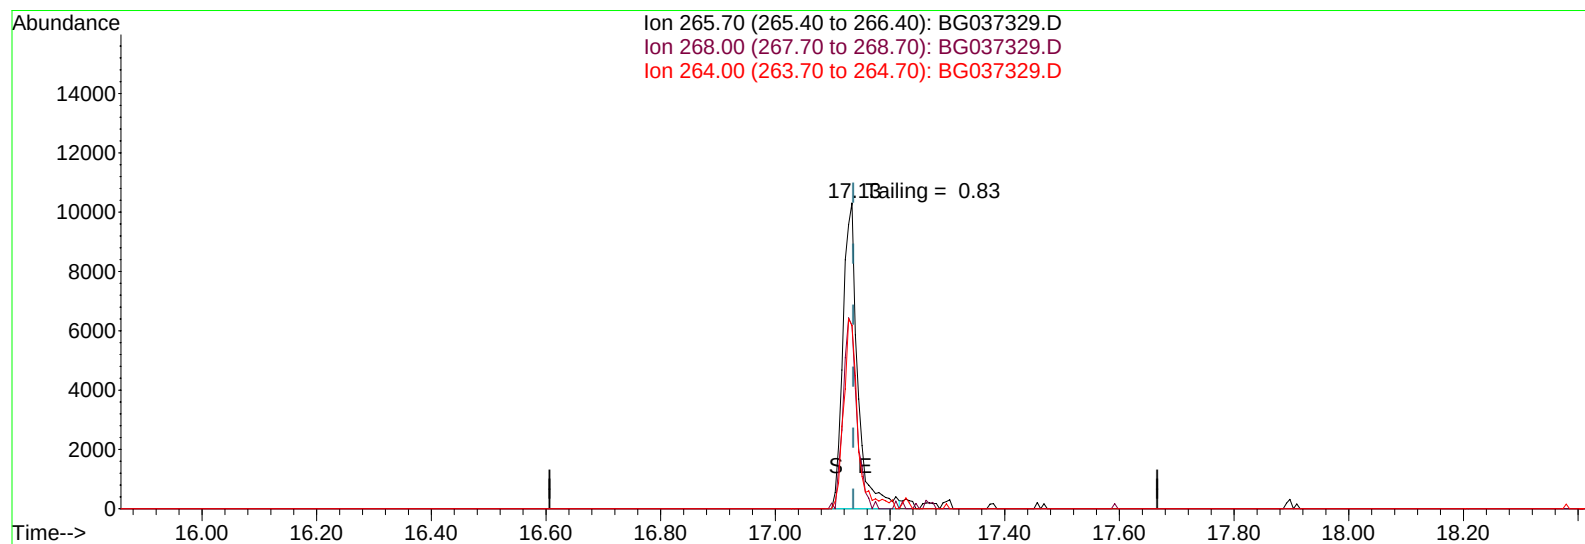

(70) Pentachlorophenol (C)

17.134min (-0.002) 7673.76ng

response 18393

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	63.65
264.00	73.60	65.19
0.00	0.00	0.00