
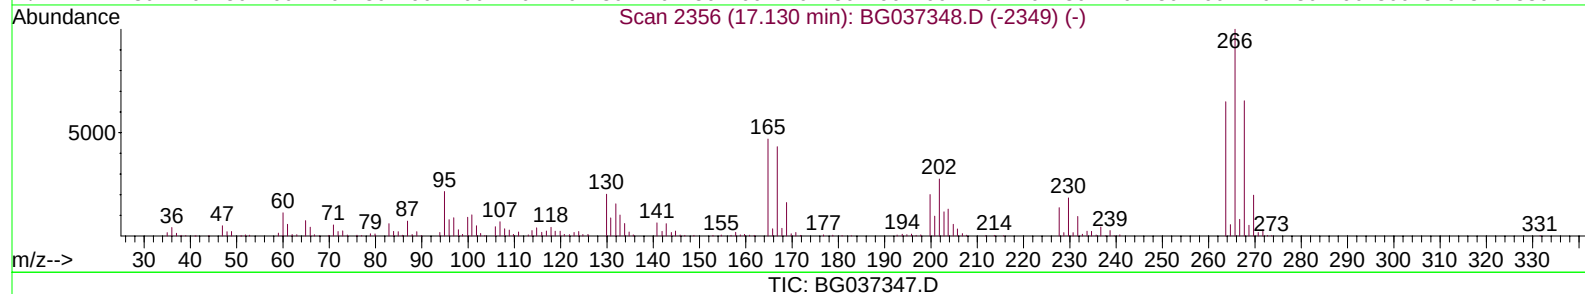
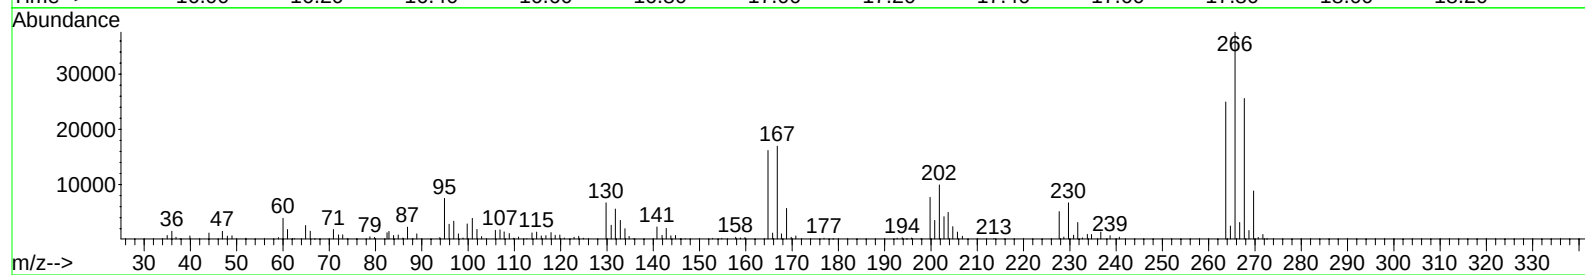


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101518\
Data File : BG037347.D
Acq On : 16 Oct 2018 00:32
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 06:57:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

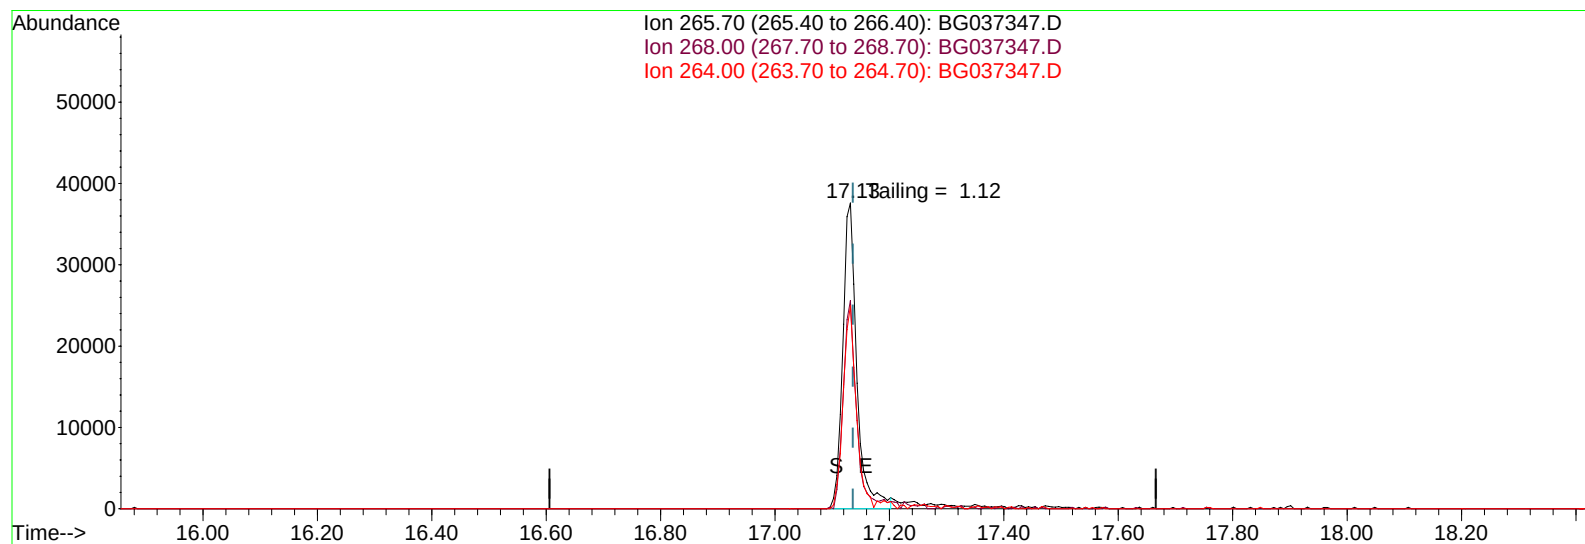

(70) Pentachlorophenol (C)




17.132min (-0.004) 16151.03ng

response 65647

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	72.57
264.00	73.60	73.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101518\
Data File : BG037347.D
Acq On : 16 Oct 2018 00:32
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 06:57:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

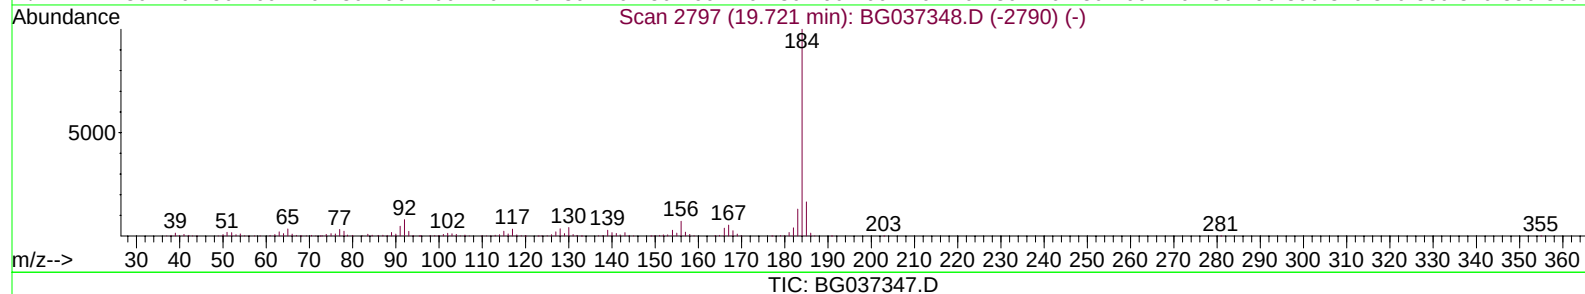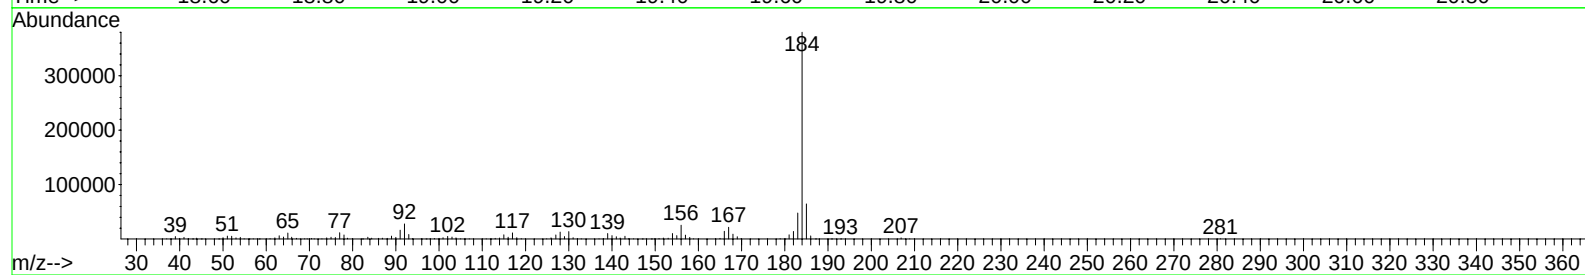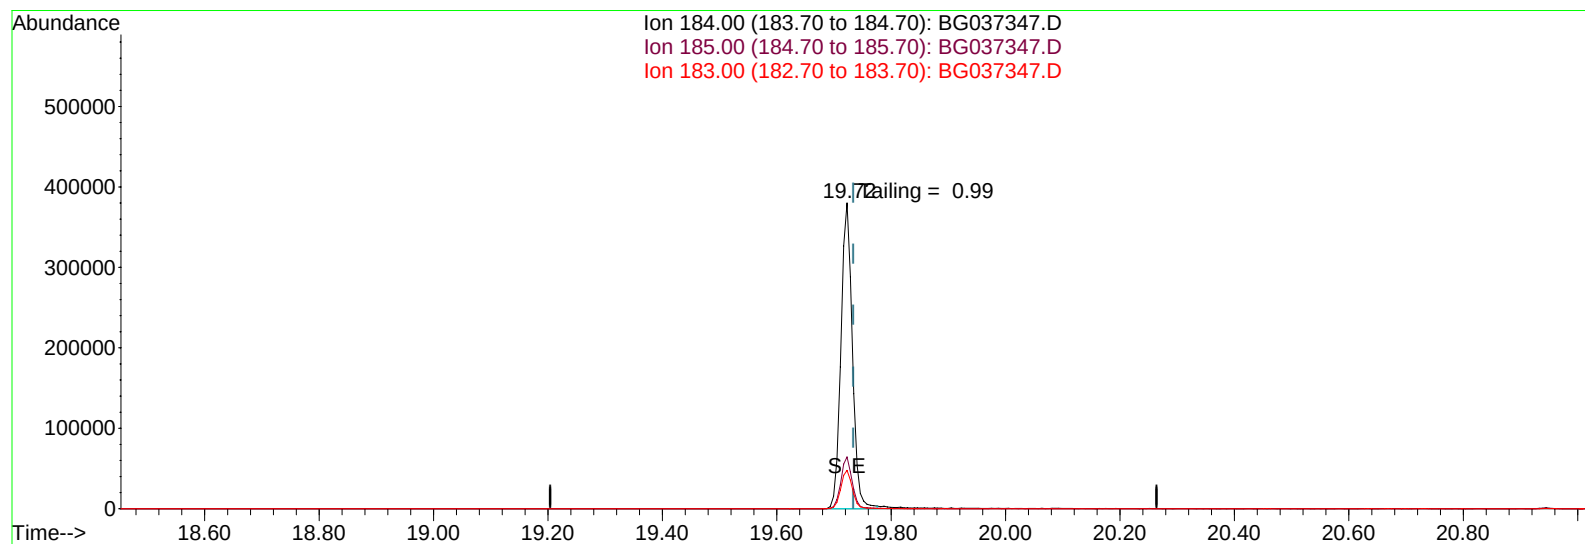

(77) Benzidine

19.723min (-0.011) 60110.44ng

response 533499

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.96
183.00	12.70	12.57
0.00	0.00	0.00