


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG101518\
Data File : BG037329.D
Acq On : 15 Oct 2018 11:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101118.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 11 13:59:58 2018

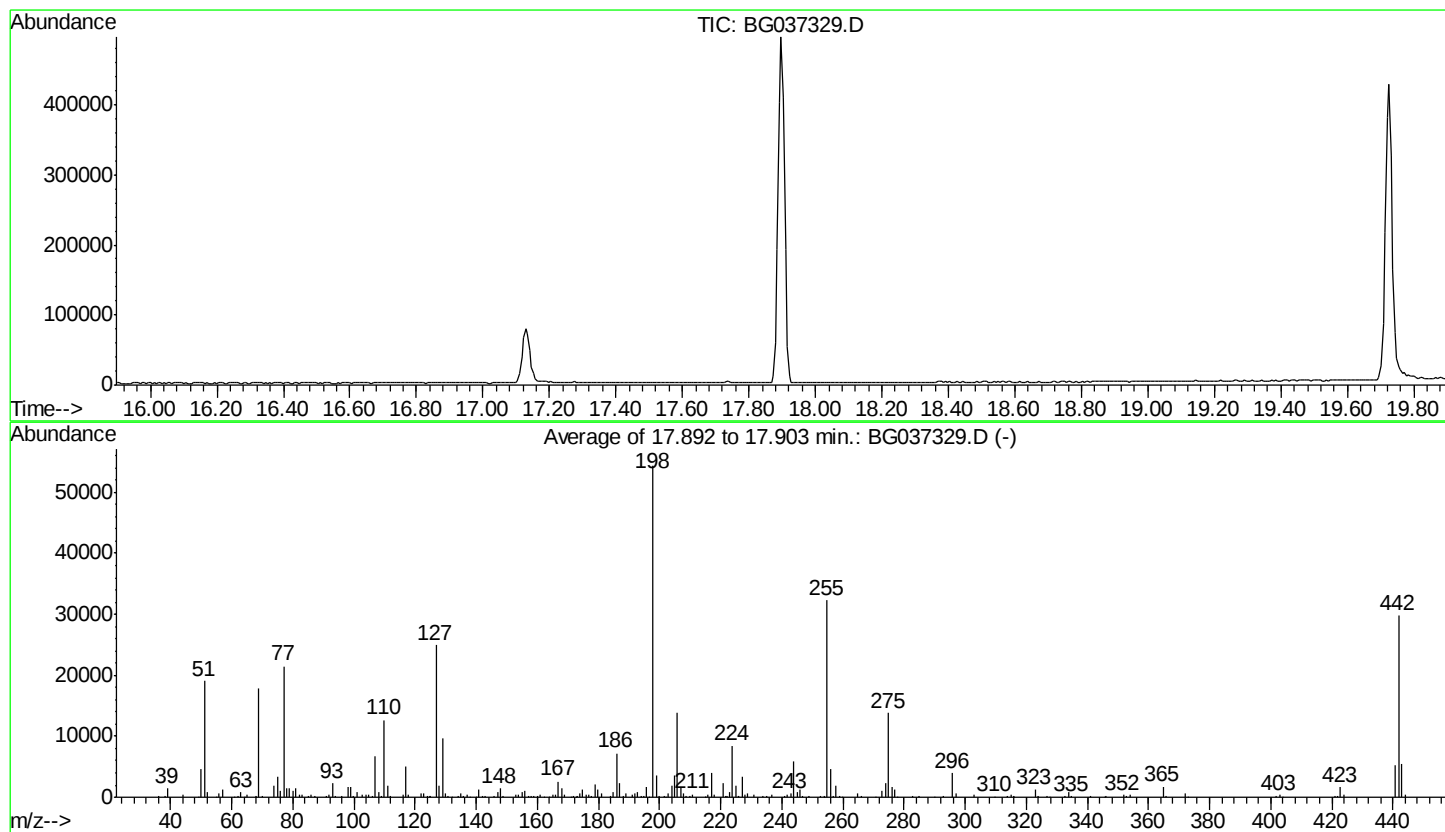

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	19030	PASS
68	69	0.00	2	1.3	234	PASS
69	198	0.00	100	32.7	17774	PASS
70	69	0.00	2	0.9	161	PASS
127	198	10	80	45.8	24898	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54378	PASS
199	198	5	9	6.4	3476	PASS
275	198	10	60	25.5	13843	PASS
365	198	1	100	3.2	1752	PASS
441	198	0.01	100	9.7	5278	PASS
442	198	50	100	54.7	29757	PASS
443	442	15	24	18.4	5465	PASS