


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG101518\
Data File : BG037347.D
Acq On : 16 Oct 2018 00:32
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101118.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 11 13:59:58 2018

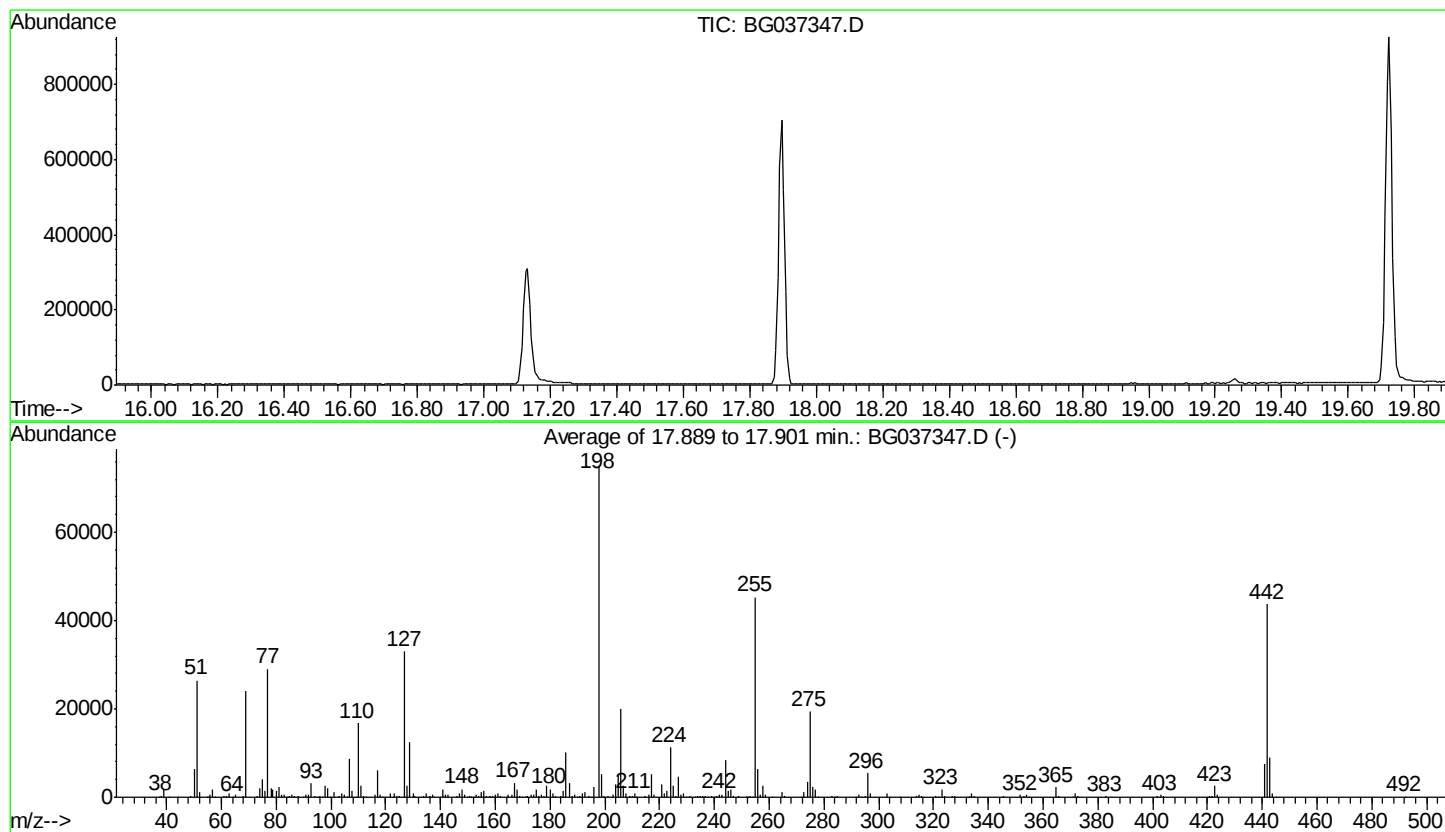

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	26484	PASS
68	69	0.00	2	0.8	190	PASS
69	198	0.00	100	32.2	24184	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.9	32992	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	75069	PASS
199	198	5	9	7.0	5265	PASS
275	198	10	60	25.8	19336	PASS
365	198	1	100	3.1	2292	PASS
441	198	0.01	100	9.9	7424	PASS
442	198	50	100	58.2	43661	PASS
443	442	15	24	20.3	8860	PASS