
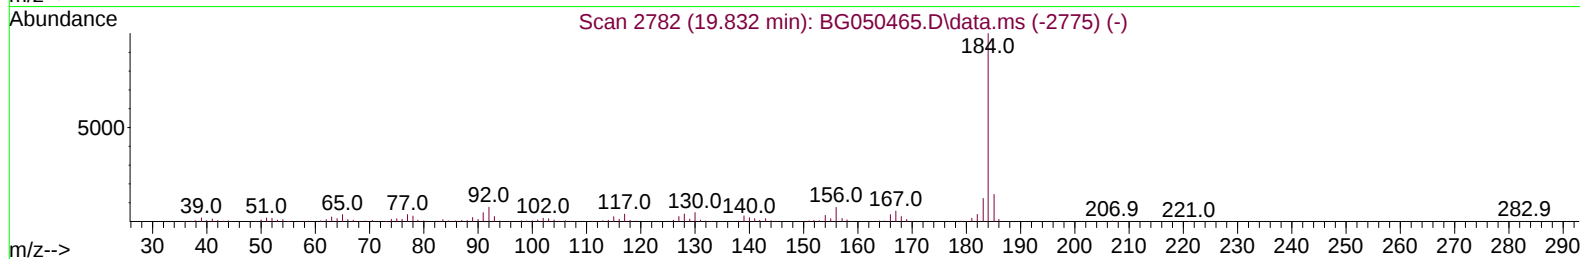
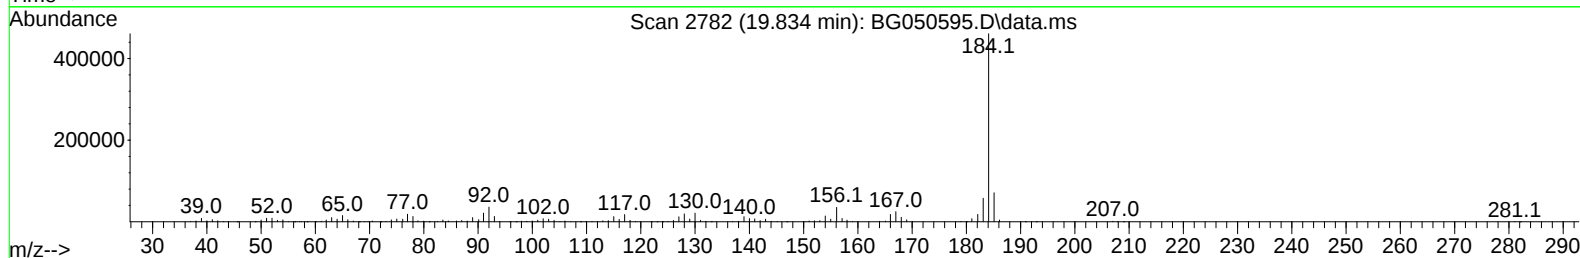


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101521\
Data File : BG050595.D
Acq On : 15 Oct 2021 9:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 18:48:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

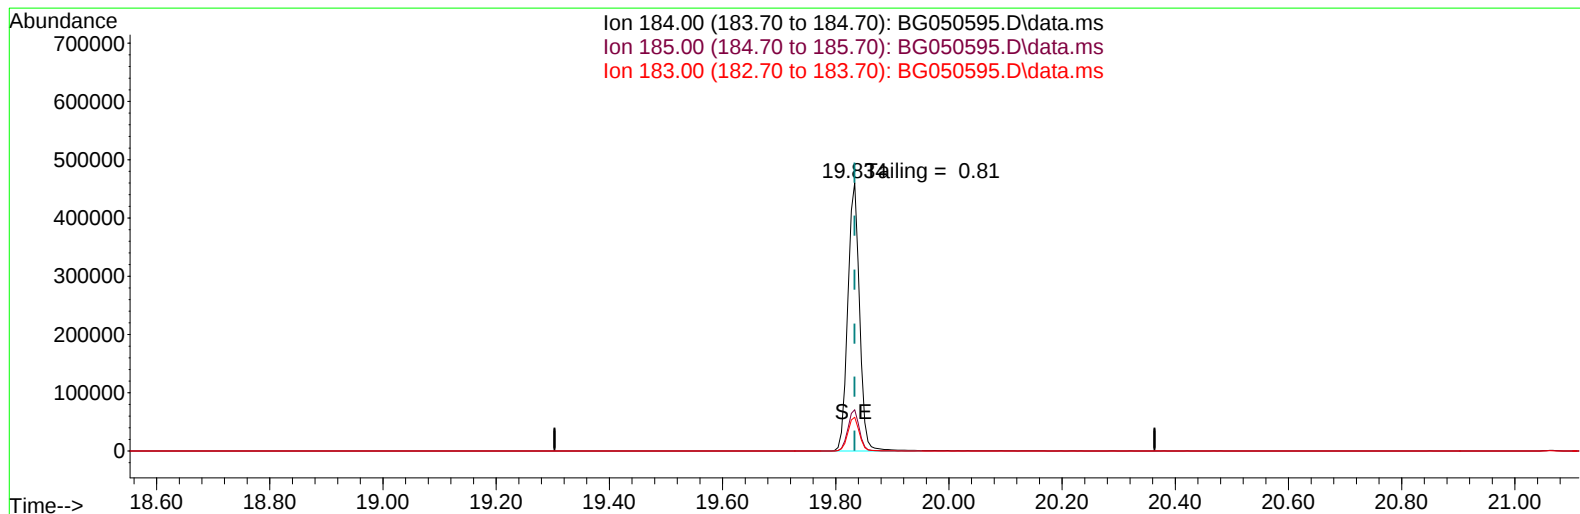




TIC: BG050595.D\data.ms

(77) Benzidine**19.834min (+ 0.001) 0.00 ng****response 660174**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.40
183.00	11.70	12.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101521\
Data File : BG050595.D
Acq On : 15 Oct 2021 9:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 18:48:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

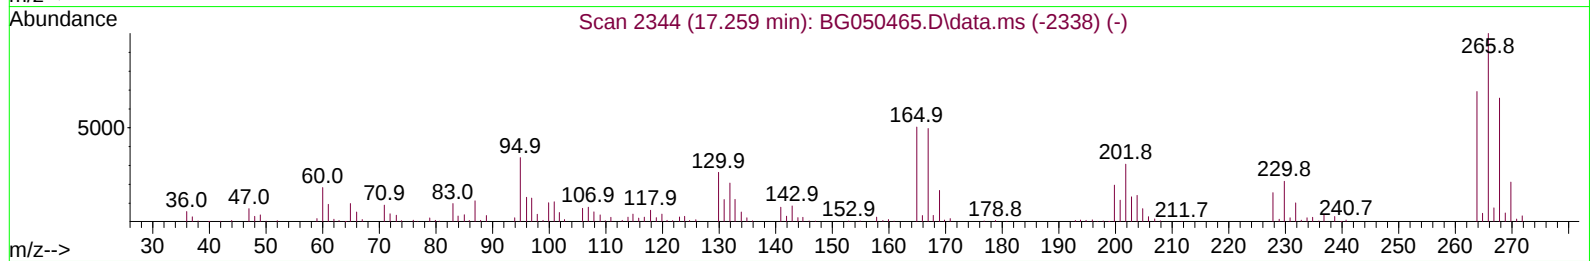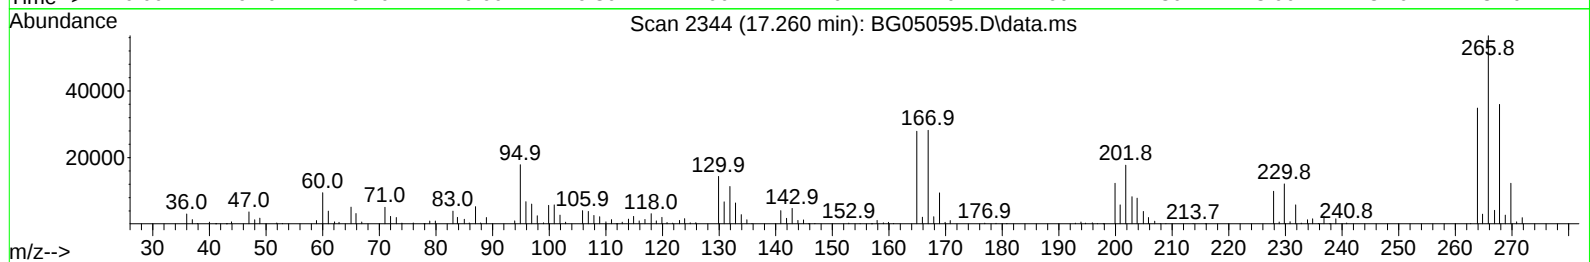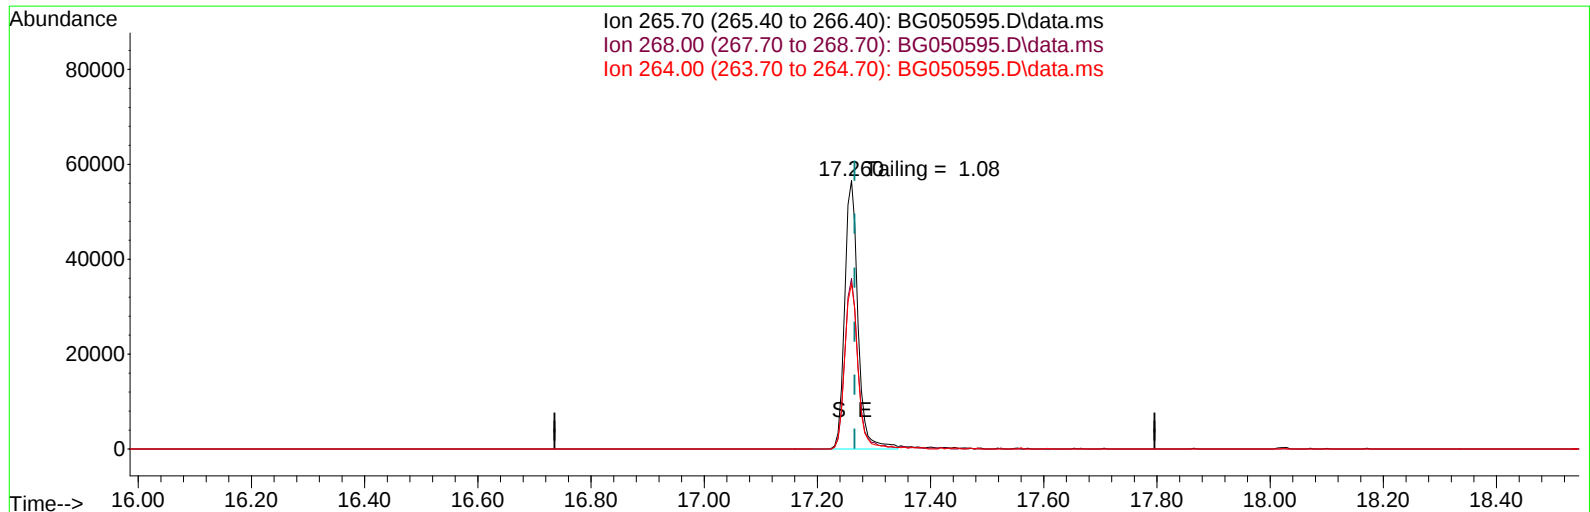

TIC: BG050595.D\data.ms

(70) Pentachlorophenol (C)

17.260min (-0.005) 23514.24 ng

response 93304

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.56
264.00	61.30	61.64
0.00	0.00	0.00