
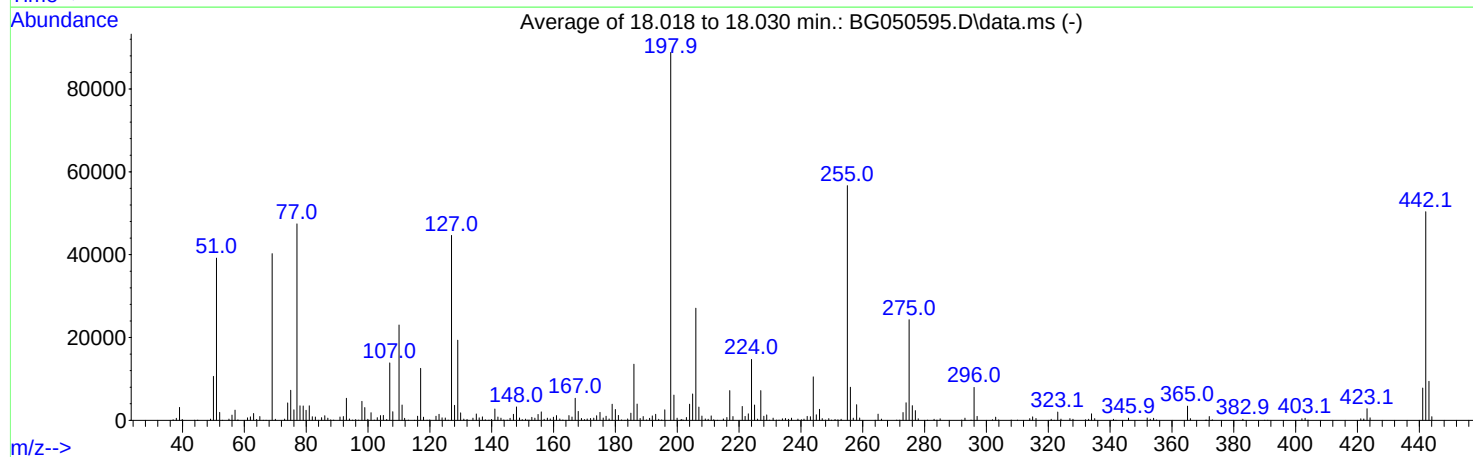


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101521\
 Data File : BG050595.D
 Acq On : 15 Oct 2021 9:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 14 10:56:22 2021

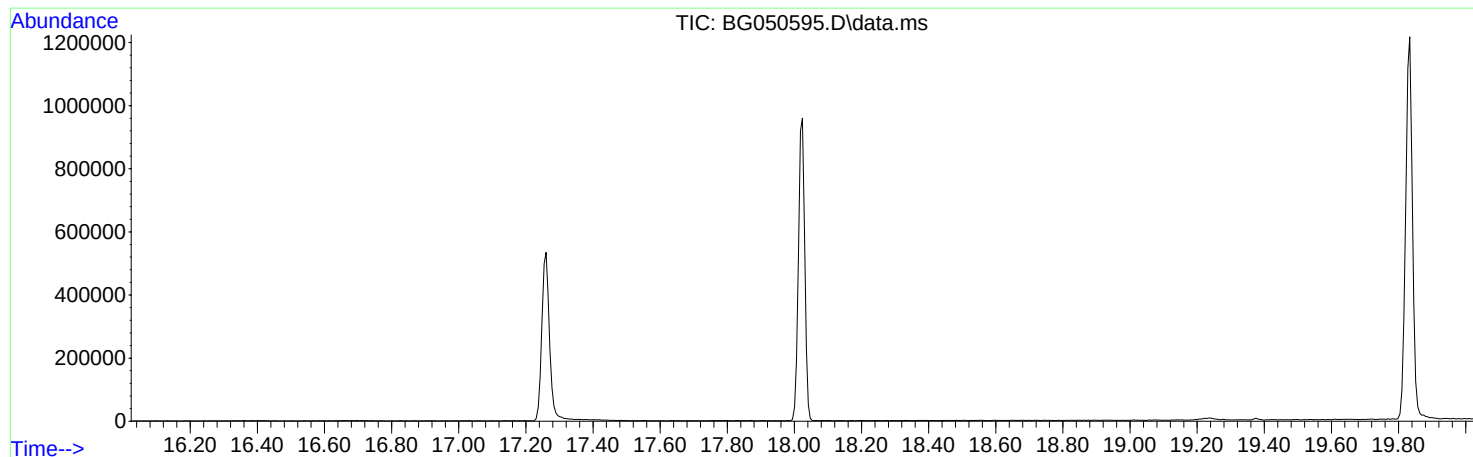




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.1	39152	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.3	40259	PASS
70	69	0.00	2	0.7	266	PASS
127	198	10	80	50.3	44637	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	88797	PASS
199	198	5	9	6.9	6097	PASS
275	198	10	60	27.4	24309	PASS
365	198	1	100	3.9	3430	PASS
441	198	0.01	100	8.8	7796	PASS
442	442	50	100	100.0	50384	PASS
443	442	15	24	18.7	9427	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101521\
Data File : BG050595.D
Acq On : 15 Oct 2021 9:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 15 18:48:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

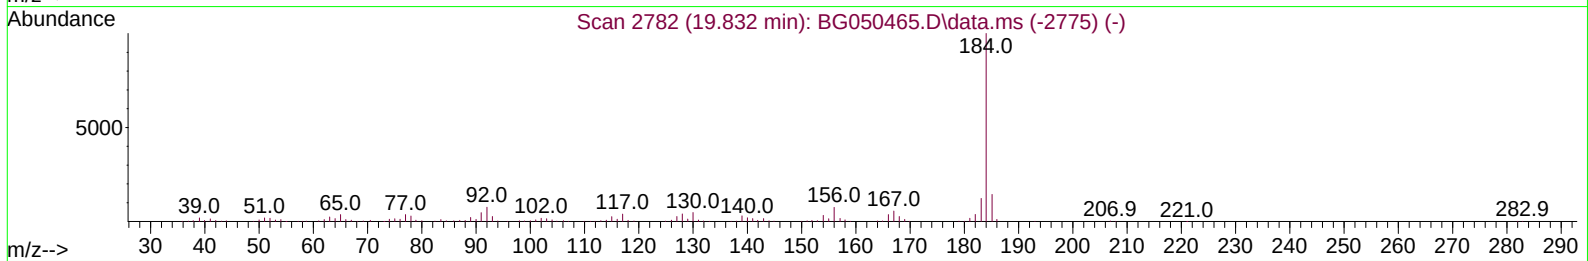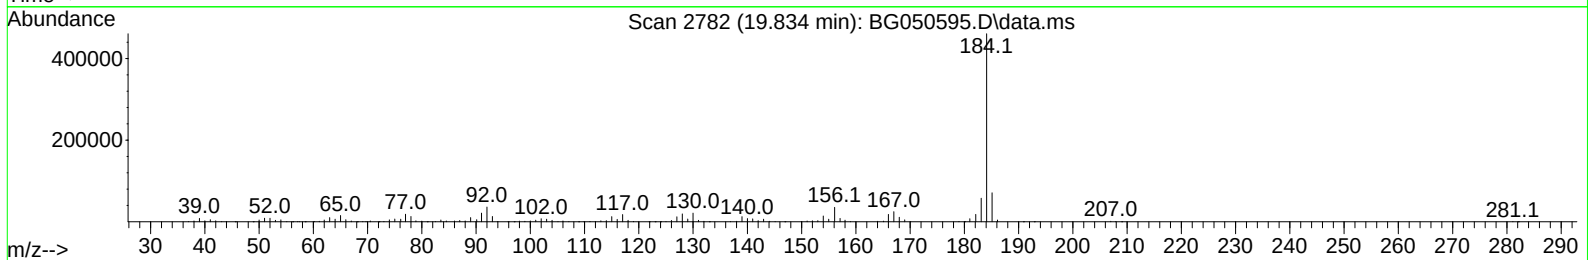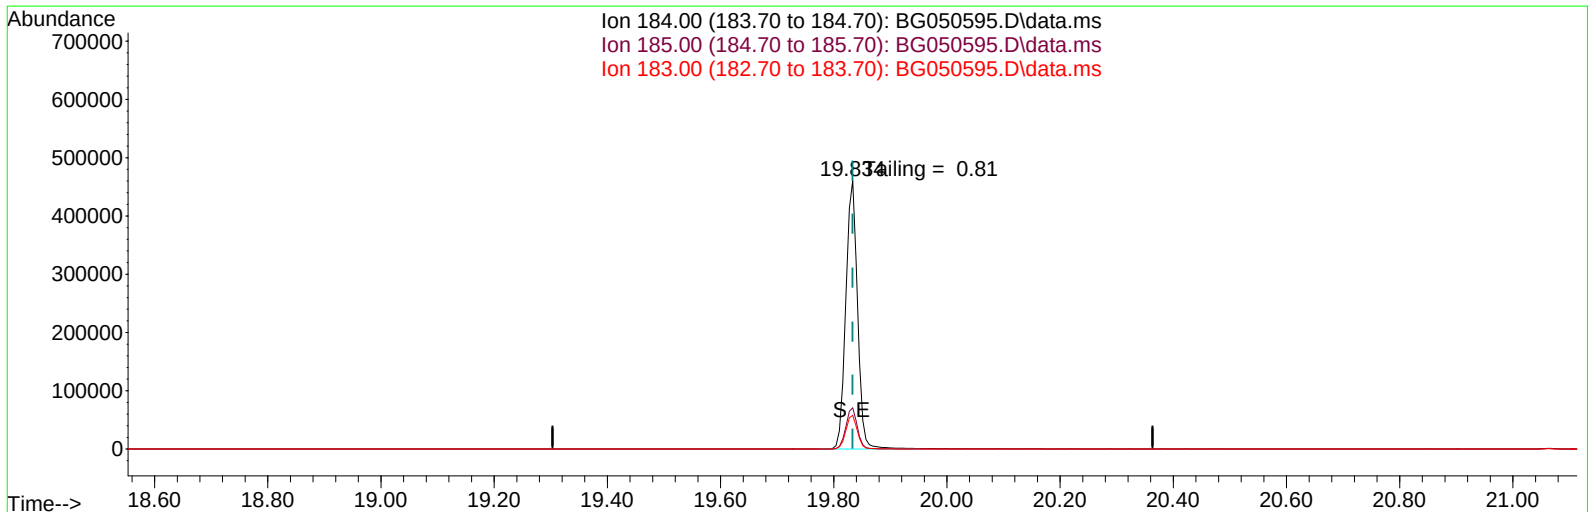

TIC: BG050595.D\data.ms

(77) Benzidine

19.834min (+ 0.001) 0.00 ng




response 660174

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.40
183.00	11.70	12.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101521\
Data File : BG050595.D
Acq On : 15 Oct 2021 9:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 15 18:48:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

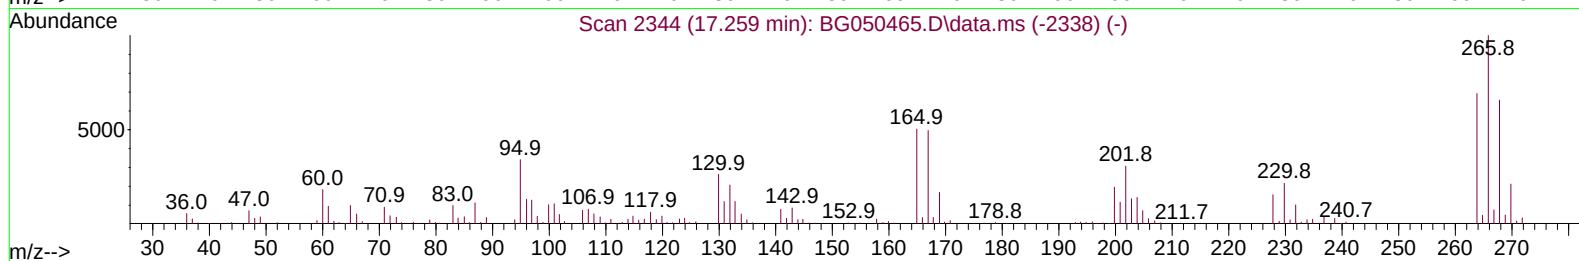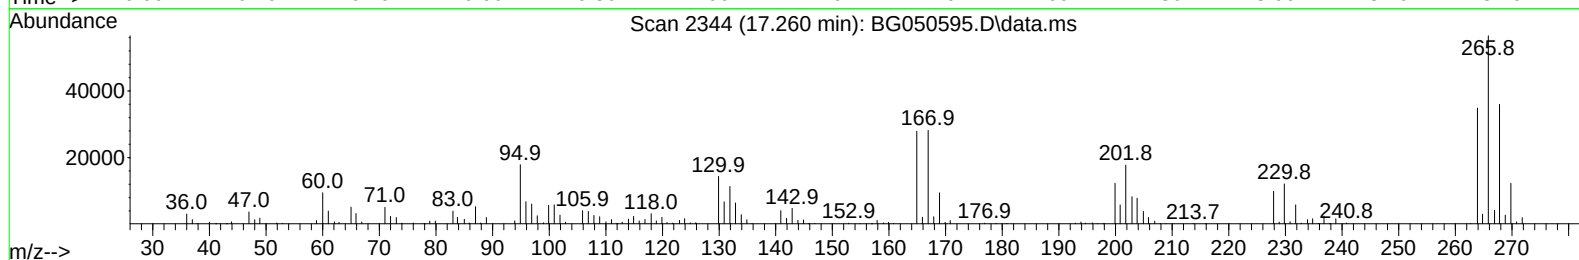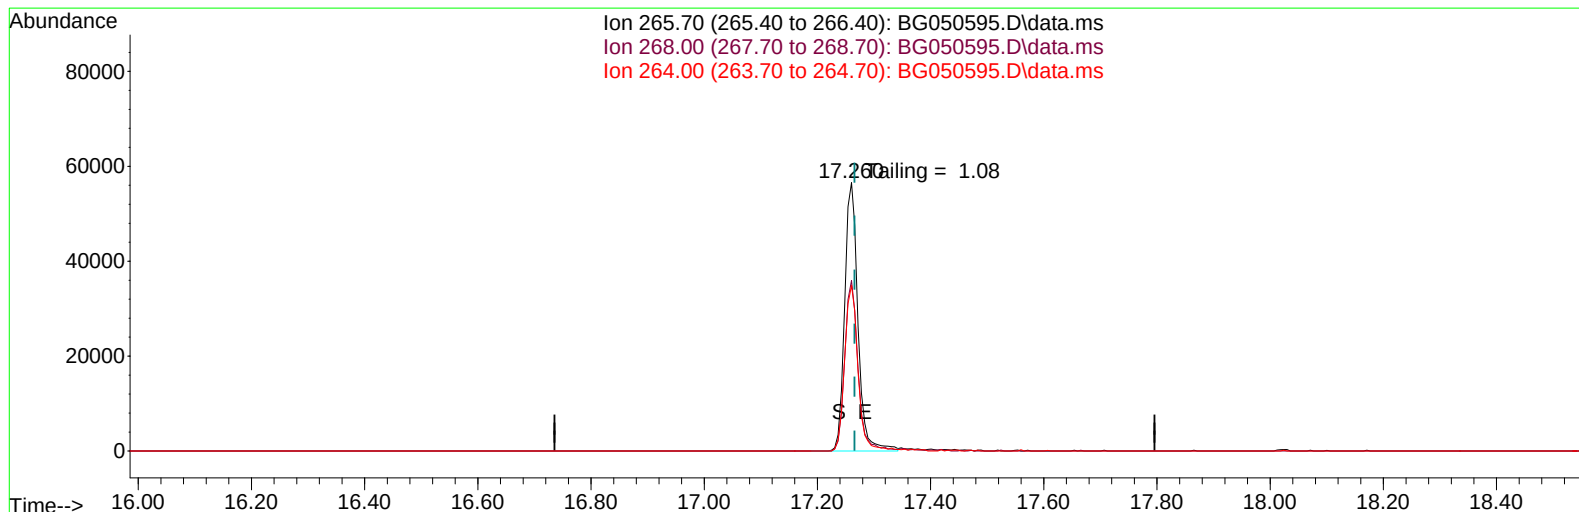

TIC: BG050595.D\data.ms

(70) Pentachlorophenol (C)

17.260min (-0.005) 23514.24 ng

response 93304

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.56
264.00	61.30	61.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/15/2021	BNA_G	BG050595.D
Compound Name	Response	Retention Time
DDT	300105	21.06
DDD	3501	20.6
DDE	1204	20.11
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4705	304810	1.54

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP