

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101615\
 Data File : BG019227.D
 Acq On : 16 Oct 2015 17:33
 Operator : UM/NP
 Sample : G3996-20
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E5LK9

Quant Time: Oct 17 06:33:57 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG101515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 17 06:30:39 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	15272	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	70521	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	51531	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.38	188	135206	20.00	ng/ul	0.00
78) Chrysene-d12	21.65	240	169625	20.00	ng/ul	0.00
86) Perylene-d12	24.85	264	165900	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.45	96	1511	5.51	ng/uL	0.00
5) Phenol-d5	7.17	99	35774	26.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	21126	24.63	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	26366	27.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	30235	26.77	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	14373	26.45	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	17544	30.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	31292	27.40	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	43514	29.58	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	128399	28.49	ng/ul	0.00
47) Acenaphthylene-d8	14.33	160	138352	28.40	ng/ul	0.00
52) 4-Nitrophenol-d4	14.83	143	18560	22.91	ng/ul	0.00
58) Fluorene-d10	15.63	176	107411	27.88	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	20079	24.07	ng/ul	0.00
71) Anthracene-d10	17.48	188	186672	29.22	ng/ul	0.00
79) Pyrene-d10	19.77	212	232199	30.18	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.63	264	256301	30.58	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.09	163	59517	13.11	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101615\
Data File : BG019227.D
Acq On : 16 Oct 2015 17:33
Operator : UM/NP
Sample : G3996-20
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E5LK9

Quant Time: Oct 17 06:33:57 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG101515.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 17 06:30:39 2015
Response via : Initial Calibration

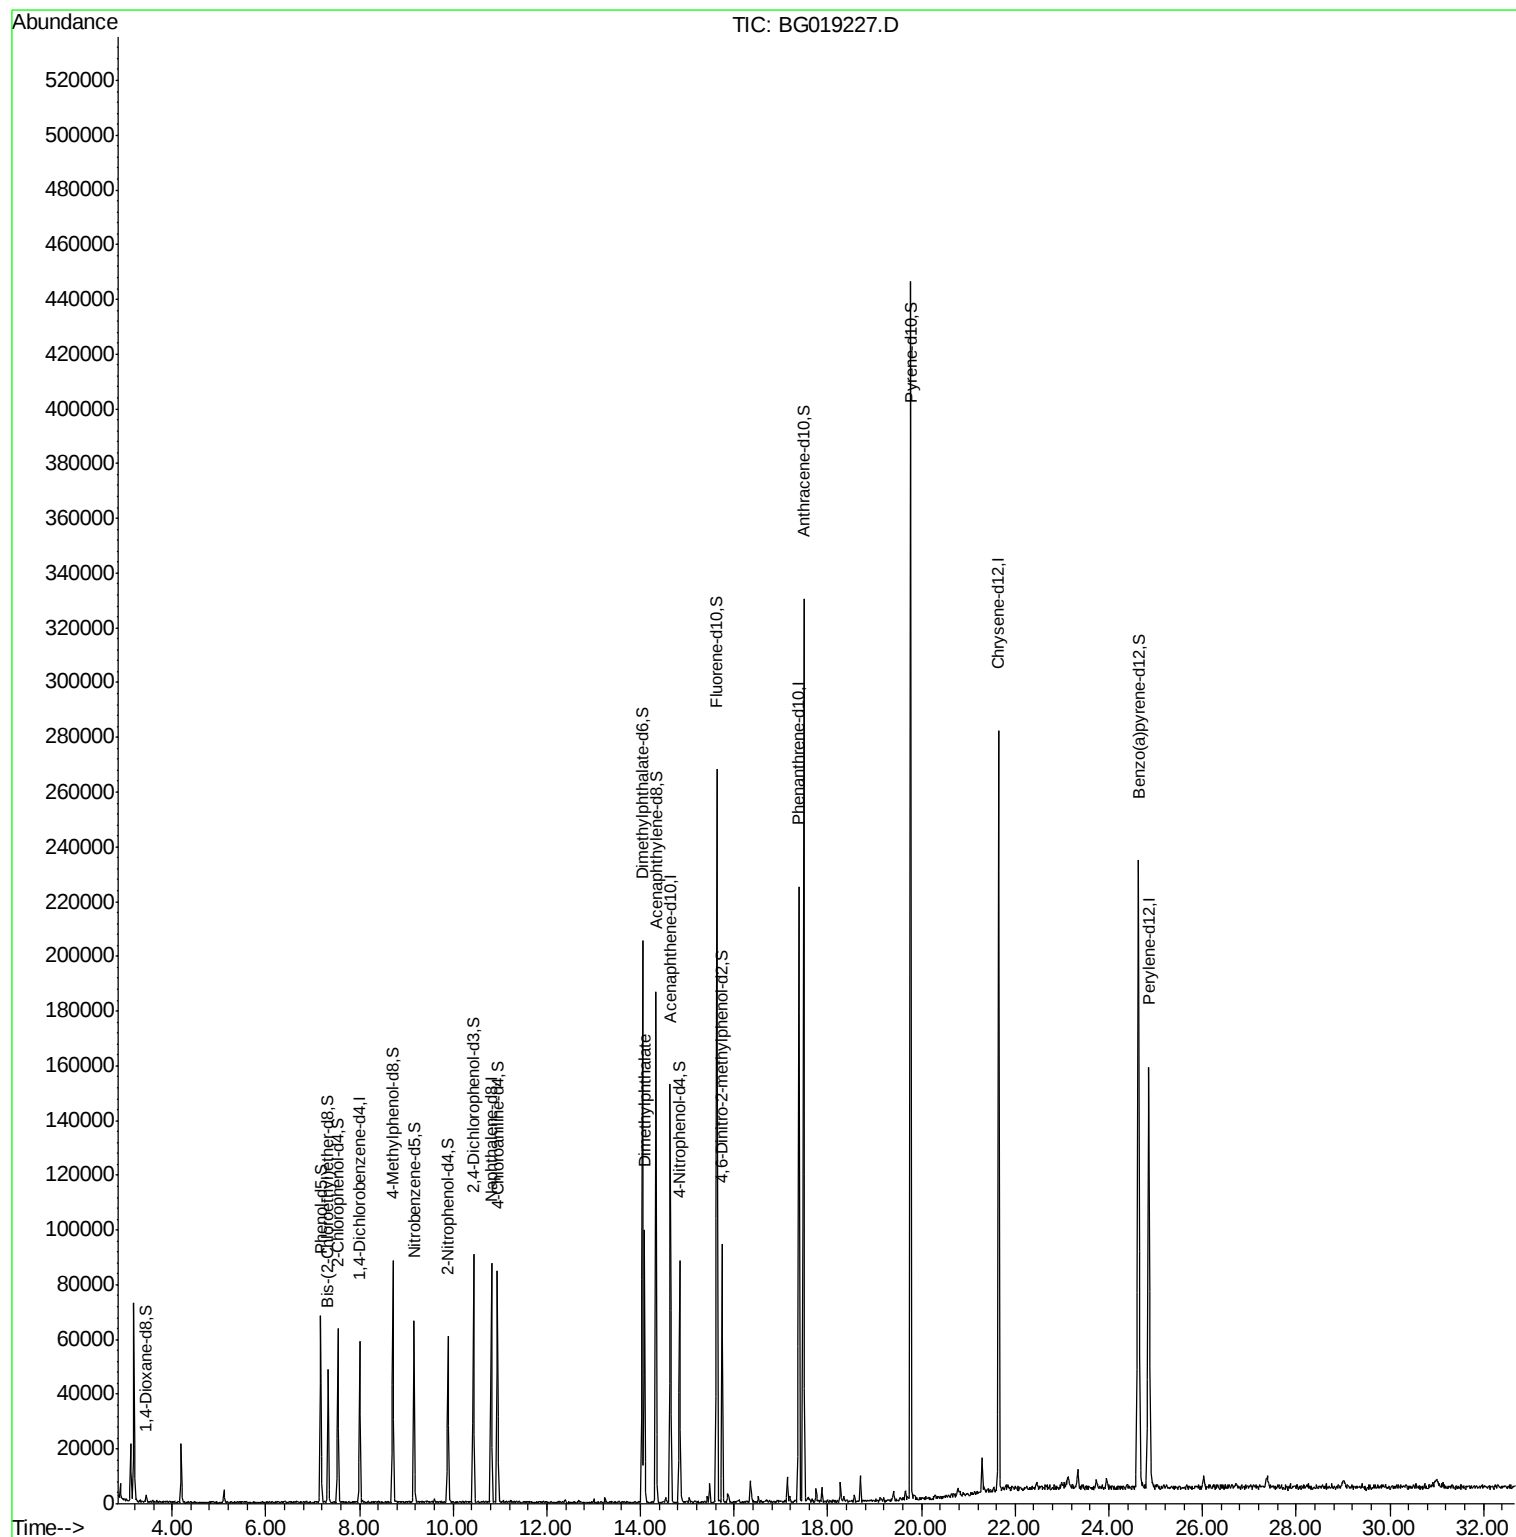

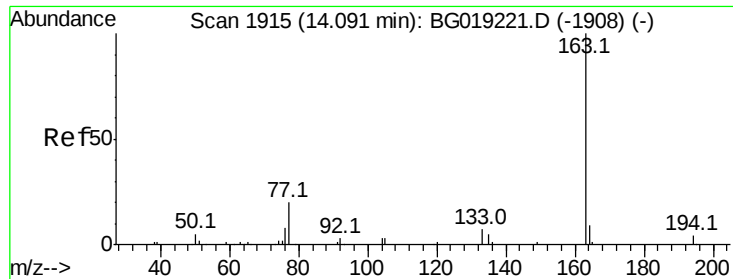

#45

Dimethylphthalate

Concen: 13.11 ng/ul

RT: 14.09 min Scan# 1914

Delta R.T. -0.00 min

Lab File: BG019227.D

Acq: 16 Oct 2015 17:33

Instrument :

BNA_G

ClientSampleId :

E5LK9


Tot Ion:163 Resp: 59517

Ion Ratio Lower Upper

163 100

194 3.8 3.3 4.9

164 9.7 8.1 12.1

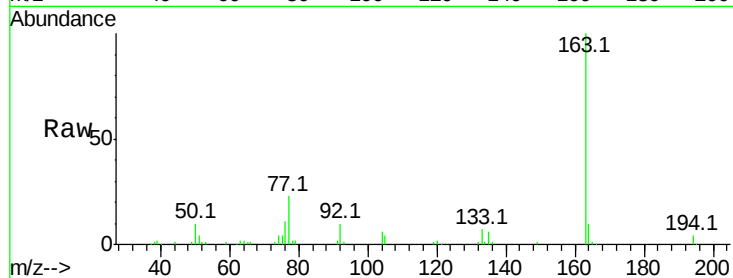

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

