

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101615\
 Data File : BG019231.D
 Acq On : 16 Oct 2015 20:05
 Operator : UM/NP
 Sample : G3996-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E5LJ8

Quant Time: Oct 17 06:34:29 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG101515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 17 06:30:39 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	15165	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	71047	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	51147	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.38	188	137442	20.00	ng/ul	0.00
78) Chrysene-d12	21.64	240	172726	20.00	ng/ul	0.00
86) Perylene-d12	24.85	264	170471	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.44	96	1107	4.07	ng/uL	0.00
5) Phenol-d5	7.17	99	28758	21.73	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	18188	21.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	21482	22.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	25326	22.59	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	12242	22.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	13174	22.68	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	25525	22.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.95	131	35753	24.13	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	102053	22.81	ng/ul	0.00
47) Acenaphthylene-d8	14.33	160	109426	22.63	ng/ul	0.00
52) 4-Nitrophenol-d4	14.83	143	19030	23.66	ng/ul	0.00
58) Fluorene-d10	15.63	176	85463	22.35	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	17058	20.12	ng/ul	0.00
71) Anthracene-d10	17.48	188	149454	23.02	ng/ul	0.00
79) Pyrene-d10	19.76	212	183886	23.47	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.63	264	207491	24.09	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.09	163	51782	11.49	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101615\
Data File : BG019231.D
Acq On : 16 Oct 2015 20:05
Operator : UM/NP
Sample : G3996-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E5LJ8

Quant Time: Oct 17 06:34:29 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG101515.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 17 06:30:39 2015
Response via : Initial Calibration

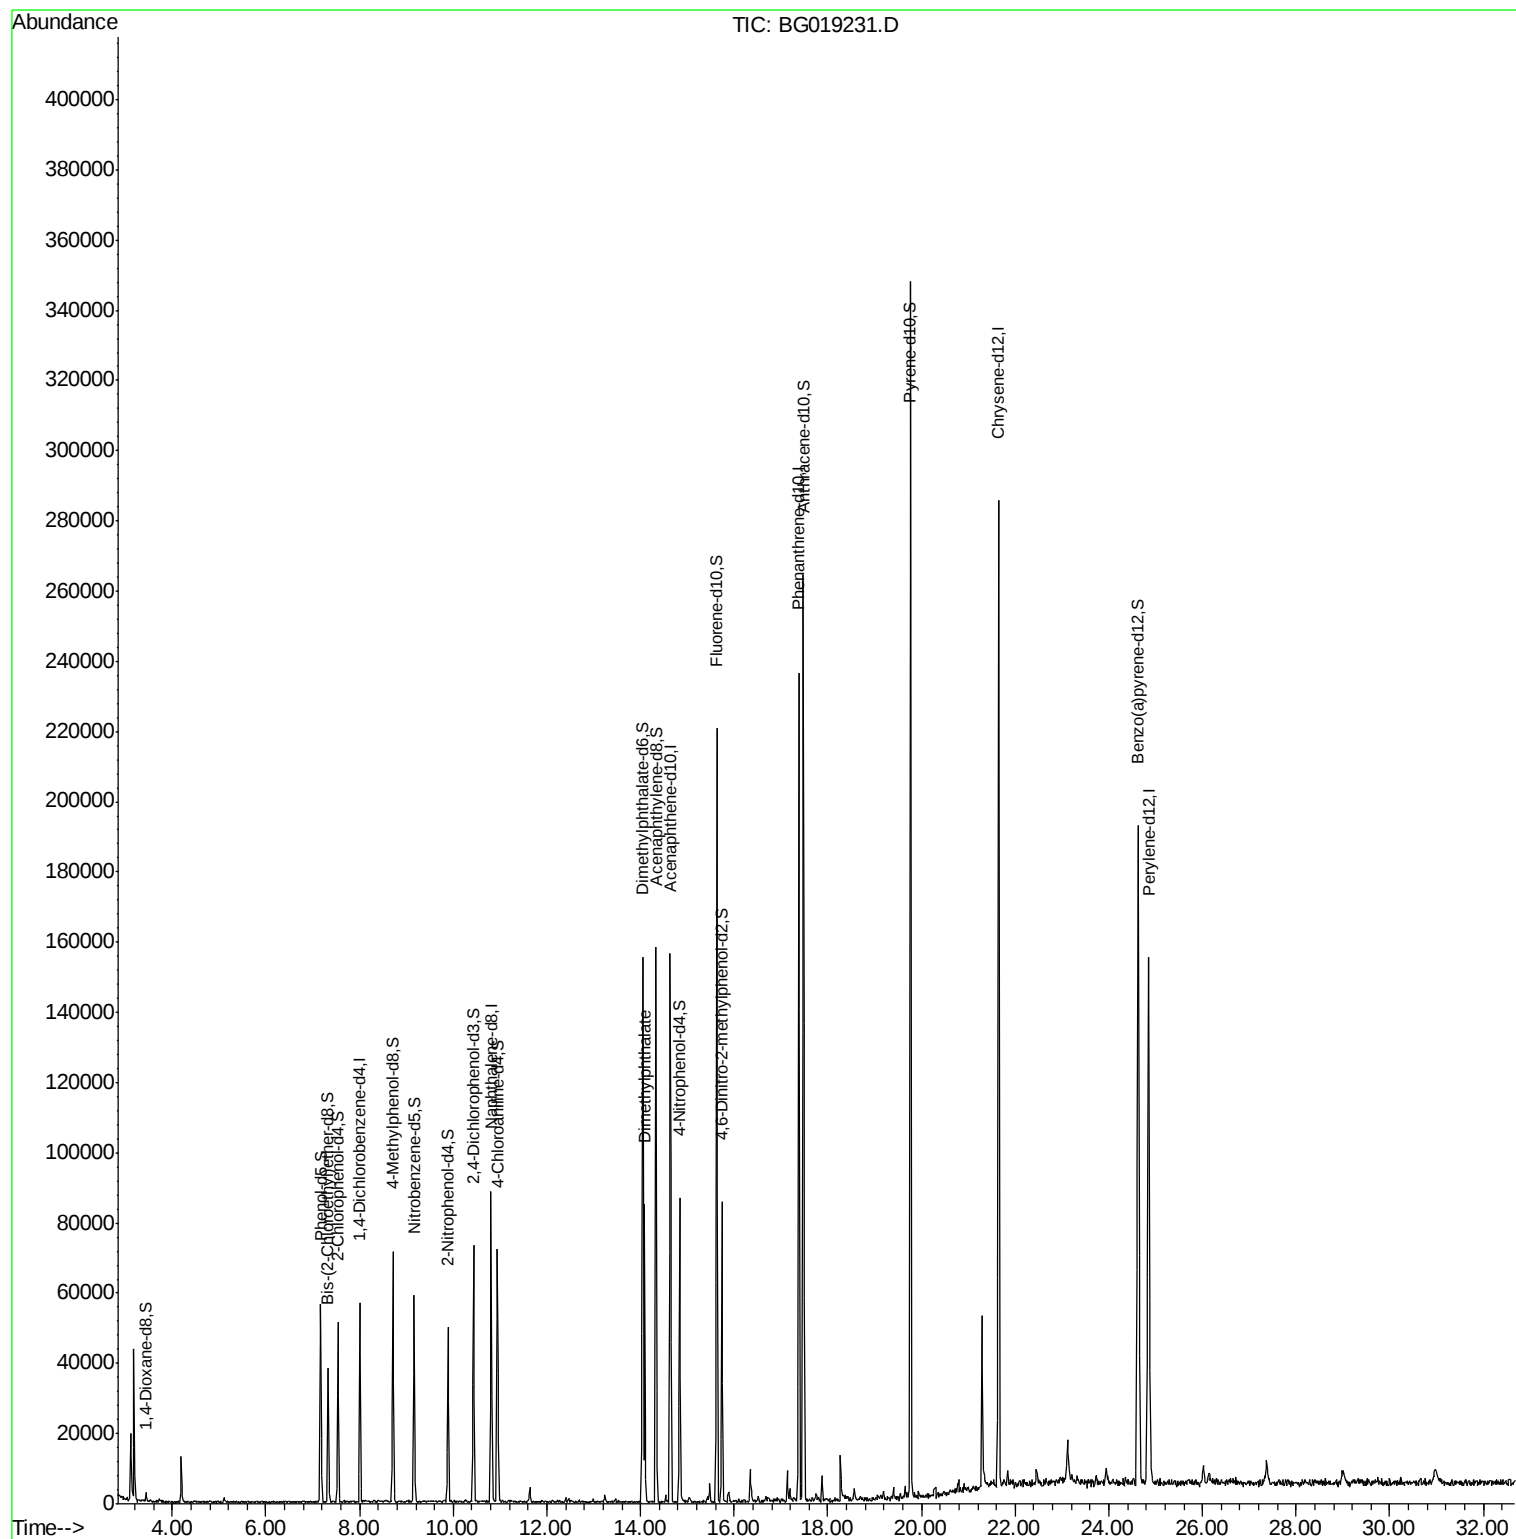

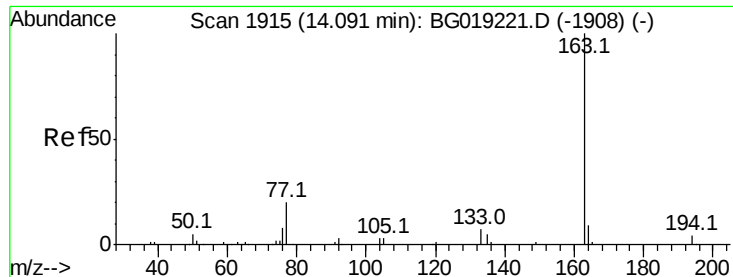

#45

Dimethylphthalate

Concen: 11.49 ng/ul

RT: 14.09 min Scan# 1915

Delta R.T. -0.00 min

Lab File: BG019231.D

Acq: 16 Oct 2015 20:05

Instrument :

BNA_G

ClientSampleId :

E5LJ8


Tot Ion:163 Resp: 51782

Ion Ratio Lower Upper

163 100

194 3.7 3.3 4.9

164 10.0 8.1 12.1

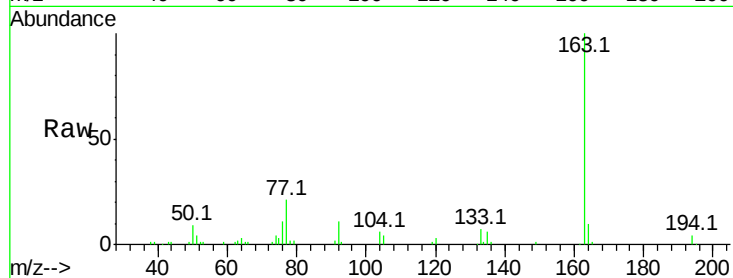

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

