

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101615\
 Data File : BG019232.D
 Acq On : 16 Oct 2015 20:43
 Operator : UM/NP
 Sample : G3996-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E5LK0

Quant Time: Oct 17 06:34:35 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG101515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 17 06:30:39 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	14775	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	69941	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	52388	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.38	188	138218	20.00	ng/ul	0.00
78) Chrysene-d12	21.65	240	172967	20.00	ng/ul	0.00
86) Perylene-d12	24.85	264	172130	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.44	96	1113	4.20	ng/uL	0.00
5) Phenol-d5	7.17	99	31757	24.63	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	19927	24.02	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	23020	24.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	26651	24.39	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	13634	25.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	15354	26.85	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	27877	24.61	ng/ul	0.00
29) 4-Chloroaniline-d4	10.95	131	39380	27.00	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	113120	24.69	ng/ul	0.00
47) Acenaphthylene-d8	14.33	160	120964	24.42	ng/ul	0.00
52) 4-Nitrophenol-d4	14.84	143	18444	22.39	ng/ul	0.00
58) Fluorene-d10	15.63	176	94827	24.21	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	17220	20.19	ng/ul	0.00
71) Anthracene-d10	17.48	188	162814	24.93	ng/ul	0.00
79) Pyrene-d10	19.77	212	201044	25.63	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.63	264	226763	26.08	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.08	163	55399	12.00	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101615\
Data File : BG019232.D
Acq On : 16 Oct 2015 20:43
Operator : UM/NP
Sample : G3996-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E5LK0

Quant Time: Oct 17 06:34:35 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG101515.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 17 06:30:39 2015
Response via : Initial Calibration

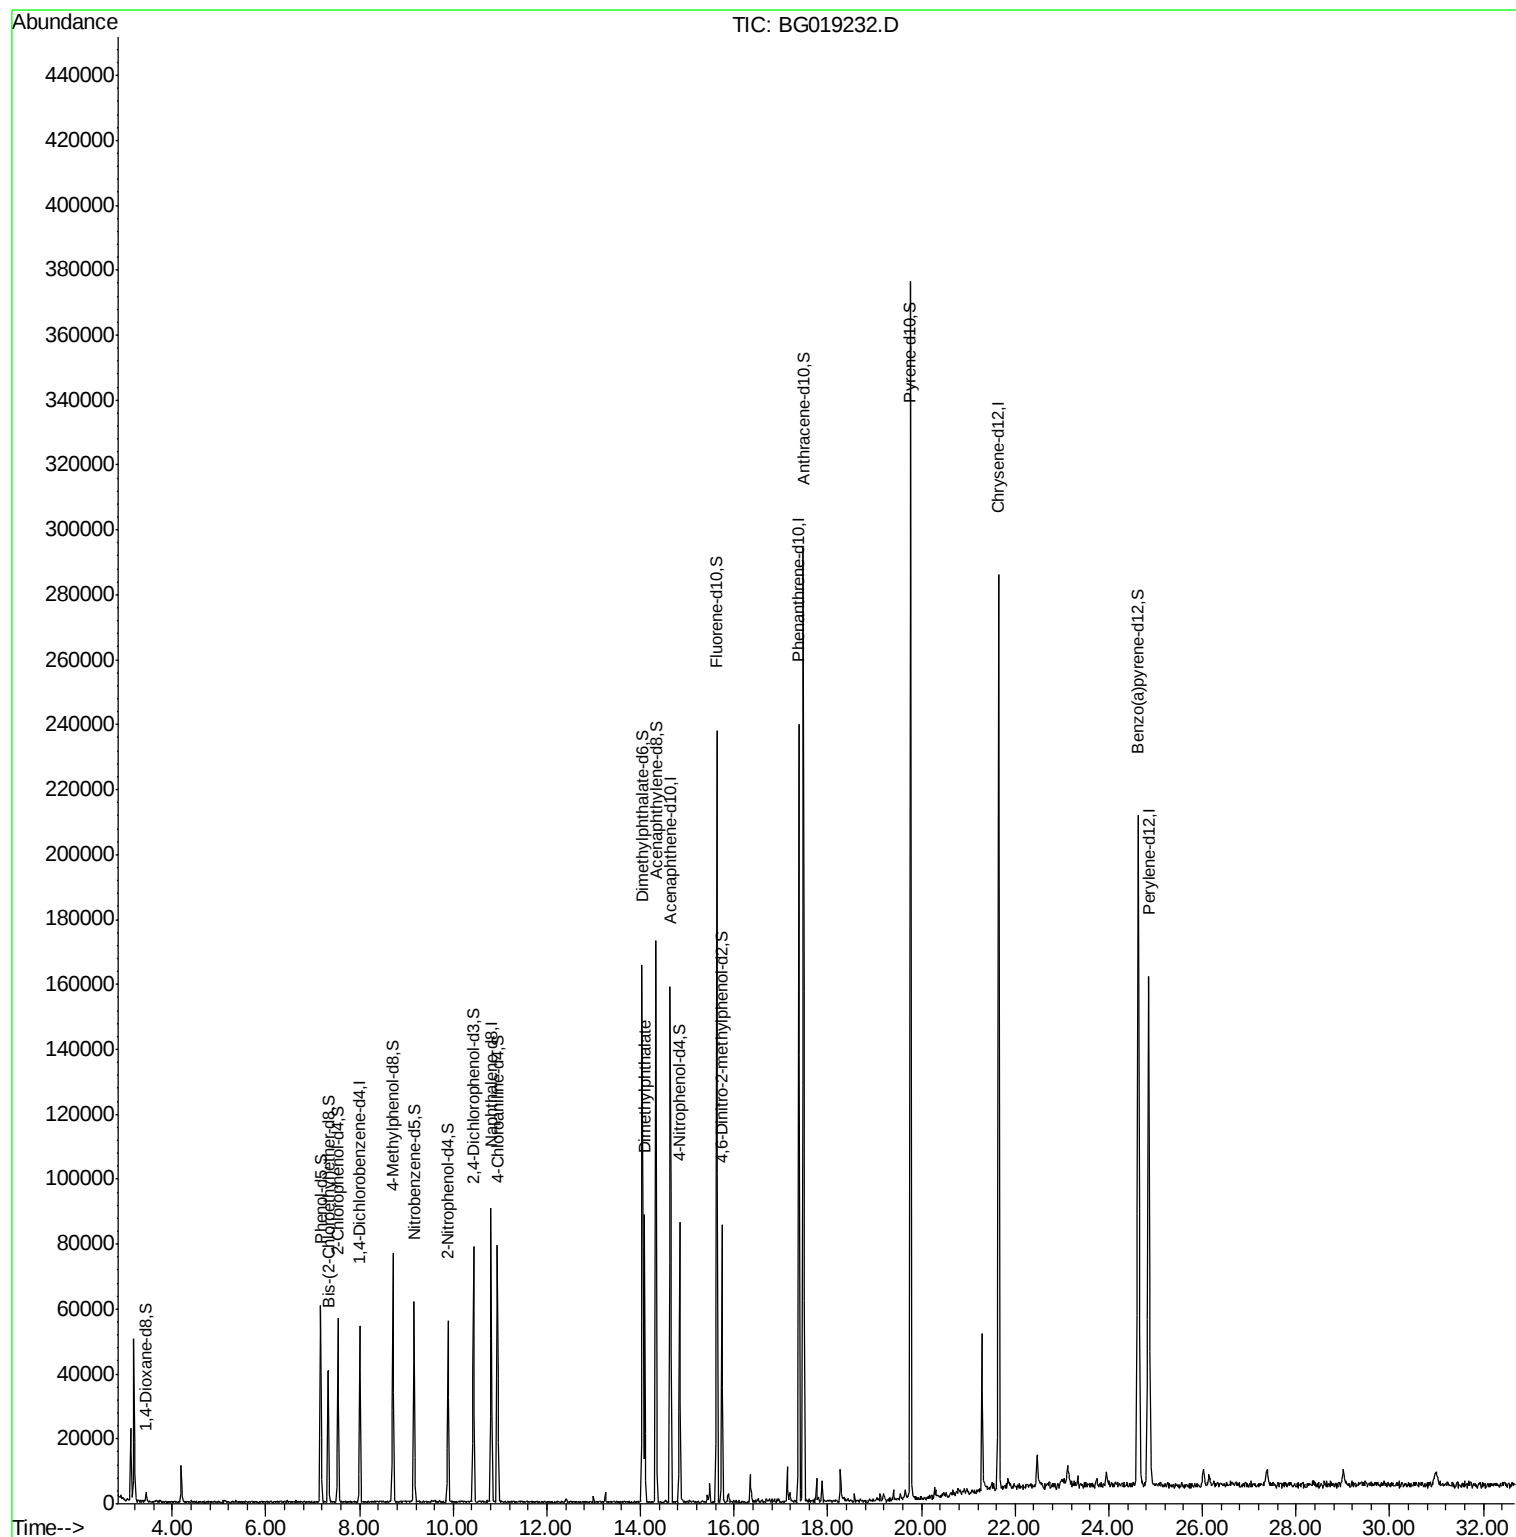

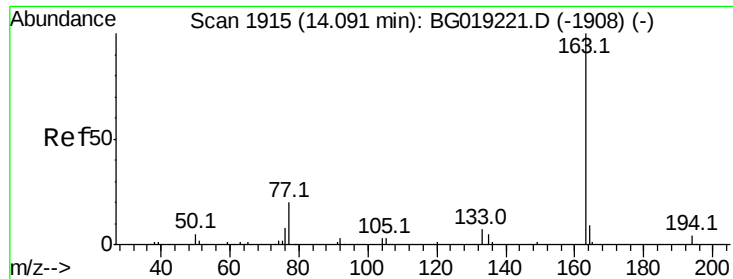

#45

Dimethylphthalate

Concen: 12.00 ng/ul

RT: 14.08 min Scan# 1914

Delta R.T. -0.01 min

Lab File: BG019232.D

Acq: 16 Oct 2015 20:43

Instrument :

BNA_G

ClientSampleId :

E5LK0


Tot Ion:163 Resp: 55399

Ion Ratio Lower Upper

163 100

194 3.3 3.3 4.9

164 10.9 8.1 12.1

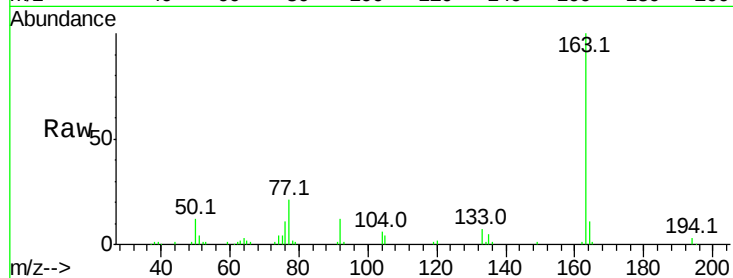

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

