
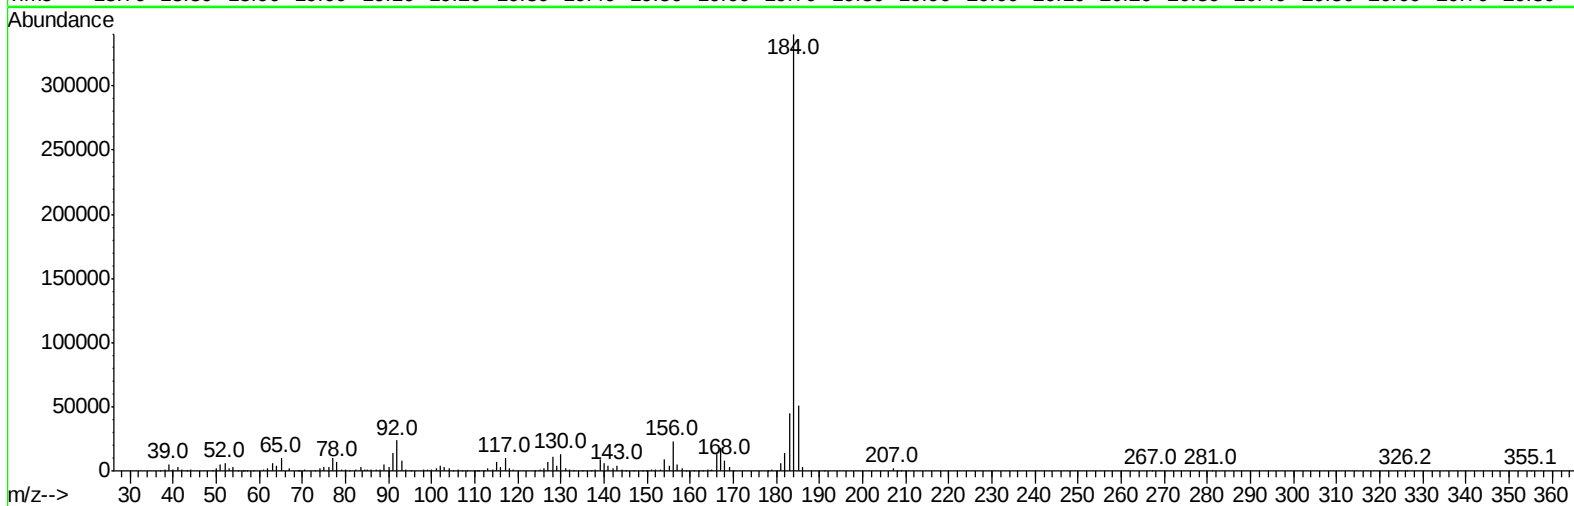


Data Path : Z:\HPCHEM1\BNA G\DATA\BG101617\
 Data File : BG029267.D
 Acq On : 16 Oct 2017 10:41
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 08:22:02 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 16 17:32:15 2017
 Response via : Initial Calibration

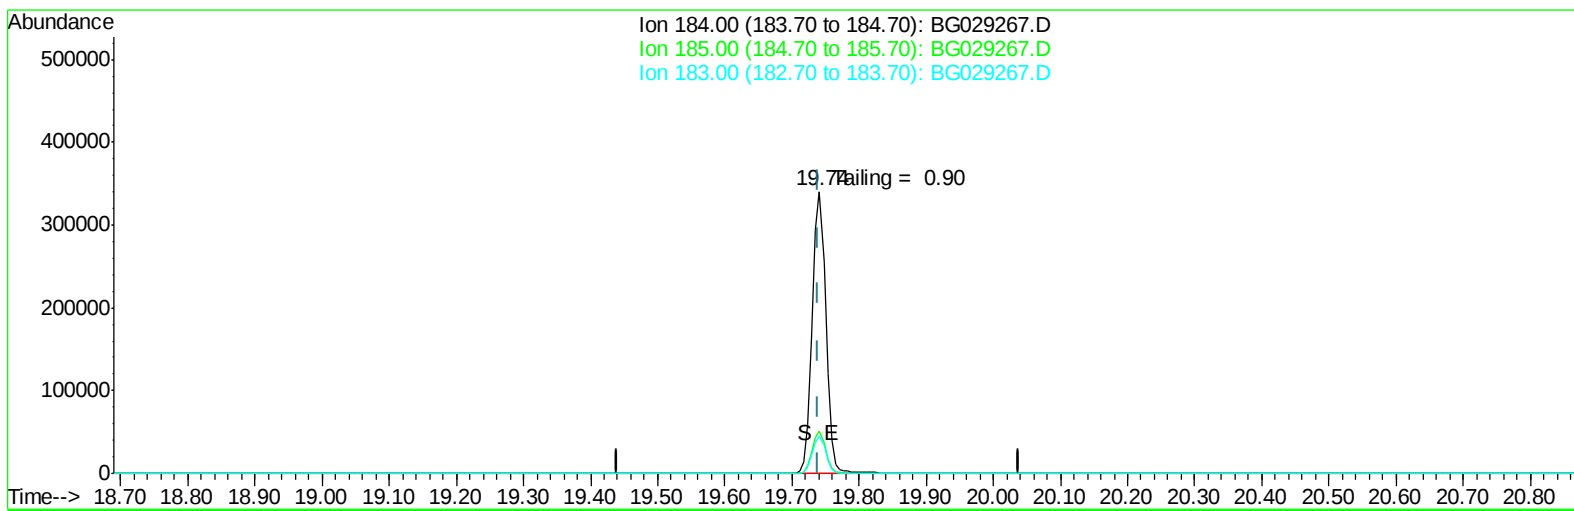

TIC: BG029267.D

(76) Benzidine



19.741min (+0.002) 53717.58ng

response 467115

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.85
183.00	13.30	13.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101617\
Data File : BG029267.D
Acq On : 16 Oct 2017 10:41
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 08:22:02 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 16 17:32:15 2017
Response via : Initial Calibration

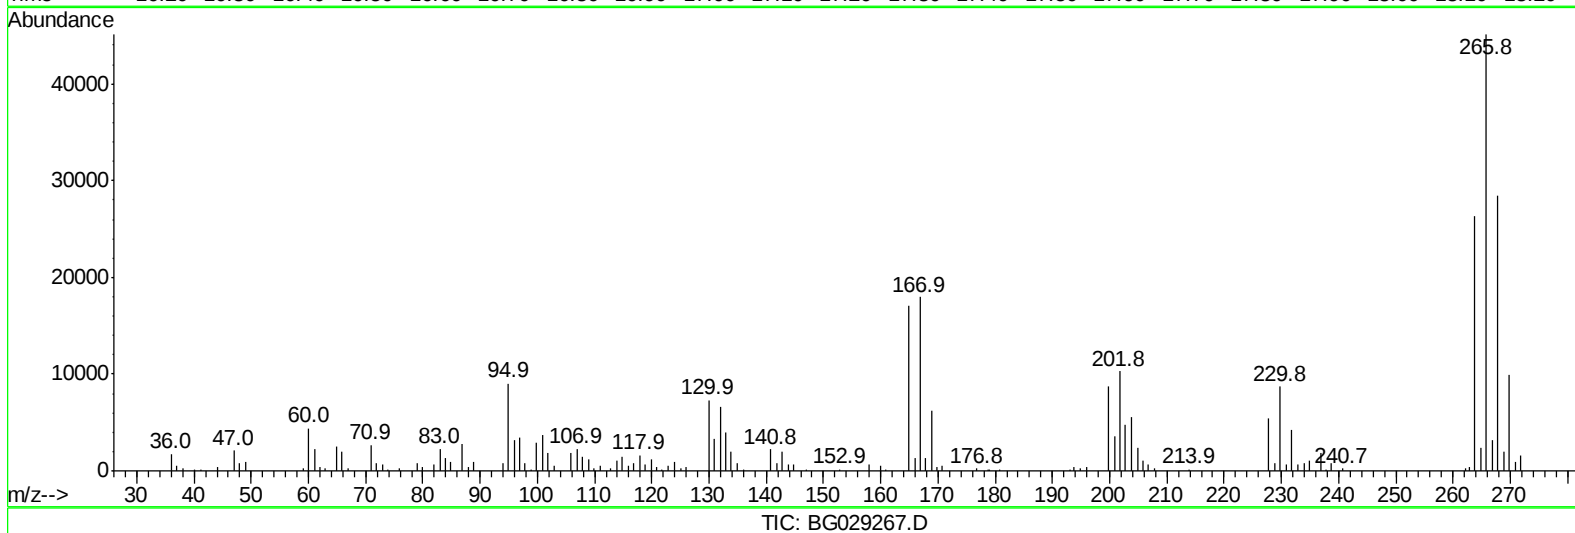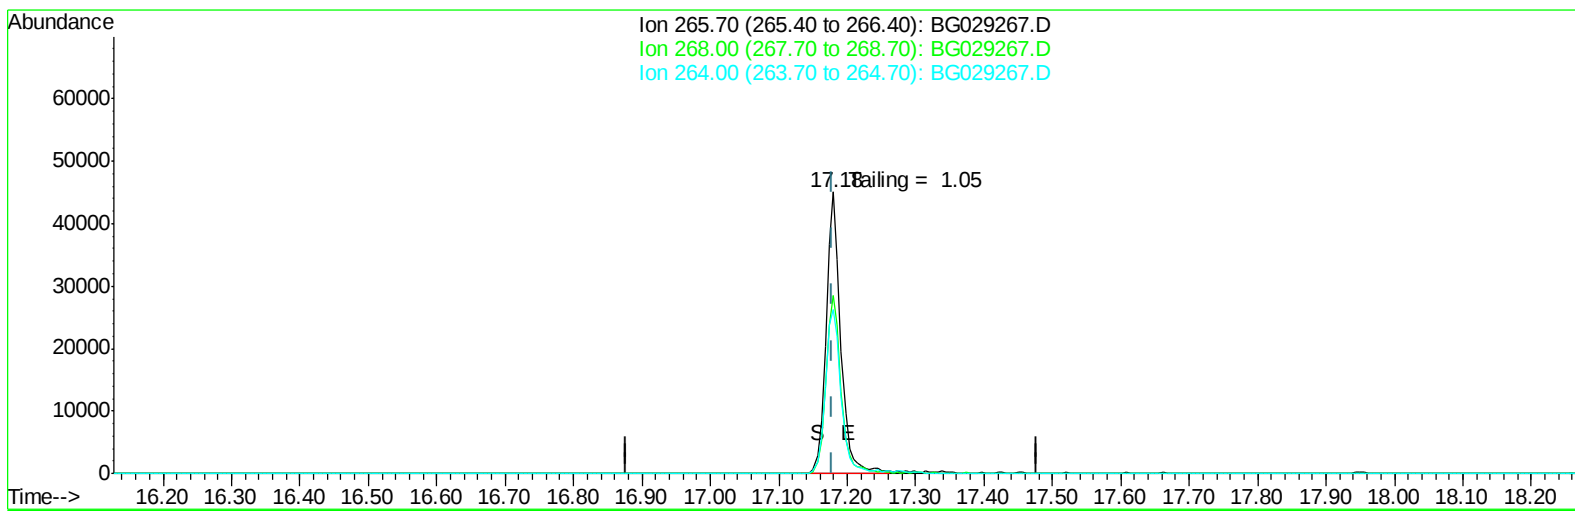

(69) Pentachlorophenol (C)

17.180min (+0.002) 157982.38ng

response 67237

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.98
264.00	62.00	58.26
0.00	0.00	0.00