
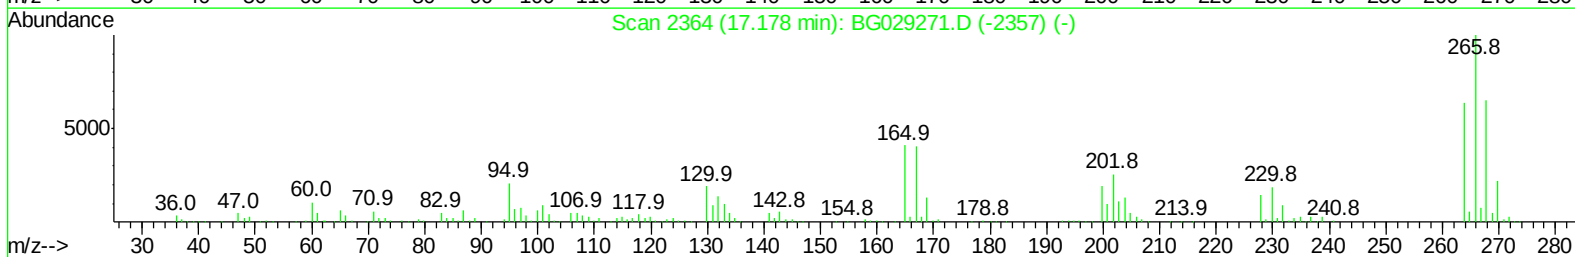
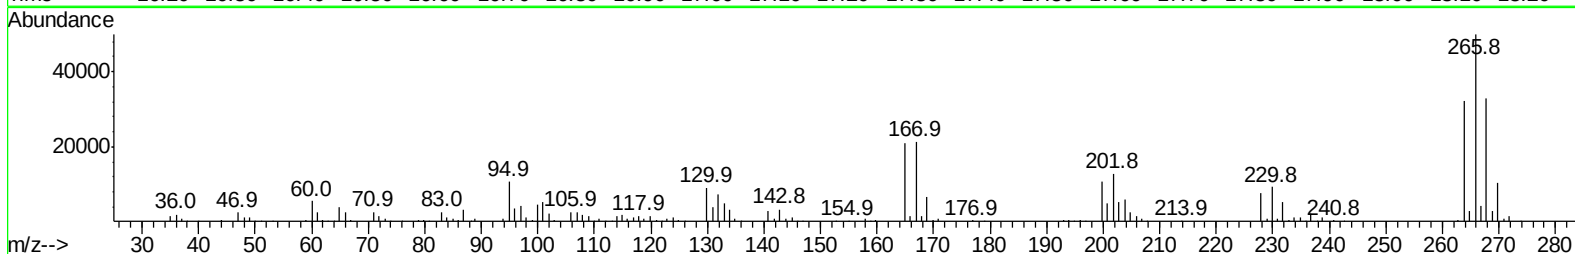


Data Path : Z:\HPCHEM1\BNA G\DATA\BG101617\
Data File : BG029281.D
Acq On : 16 Oct 2017 21:28
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 08:22:56 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 16 17:32:15 2017
Response via : Initial Calibration

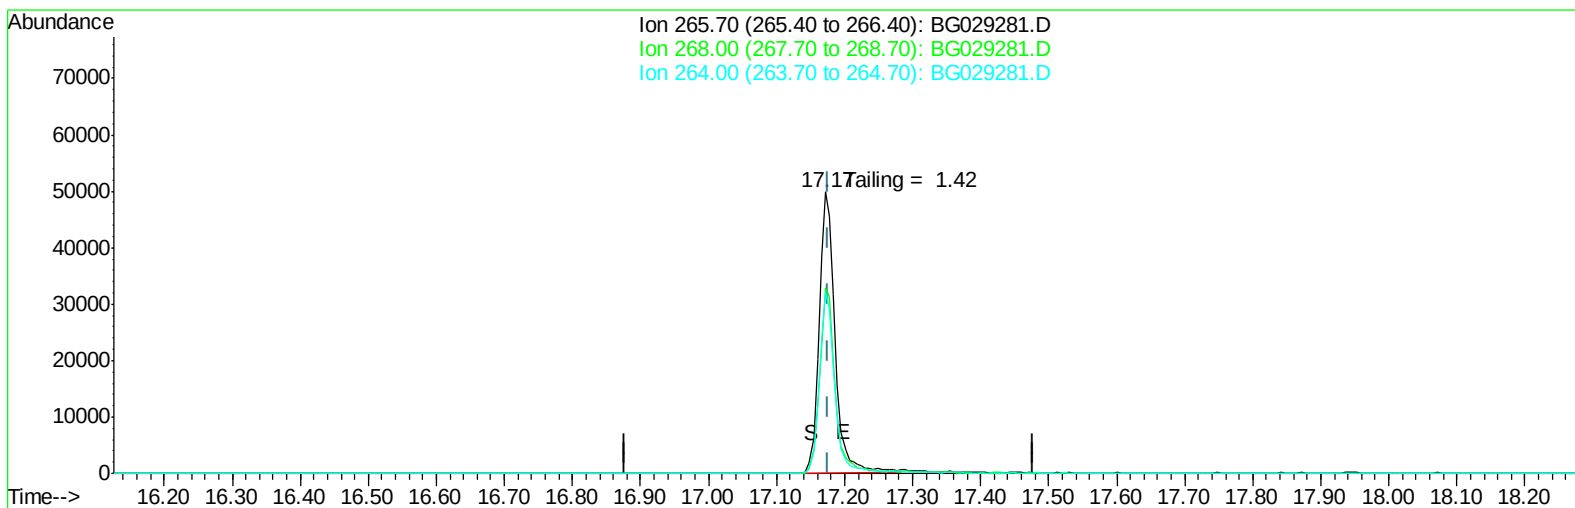

TIC: BG029281.D

(69) Pentachlorophenol (C)




17.172min (-0.006) 0.00ng

response 83051

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.96
264.00	62.00	64.58
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101617\
Data File : BG029281.D
Acq On : 16 Oct 2017 21:28
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 08:22:56 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 16 17:32:15 2017
Response via : Initial Calibration

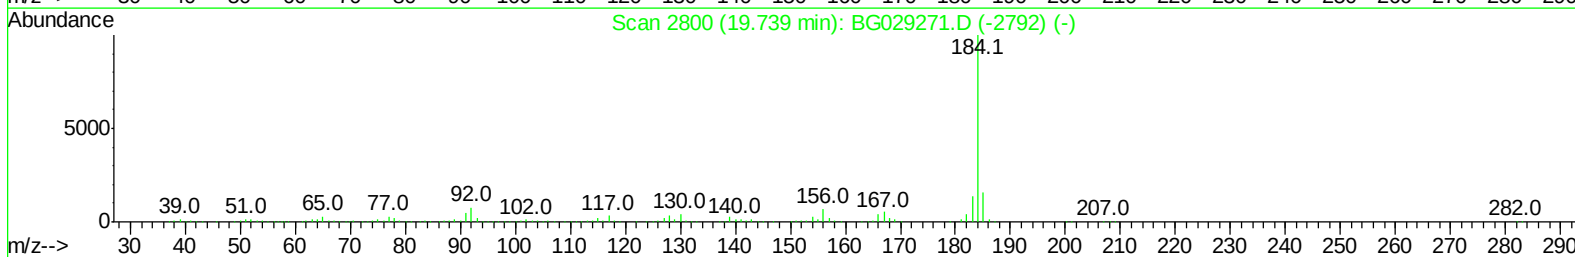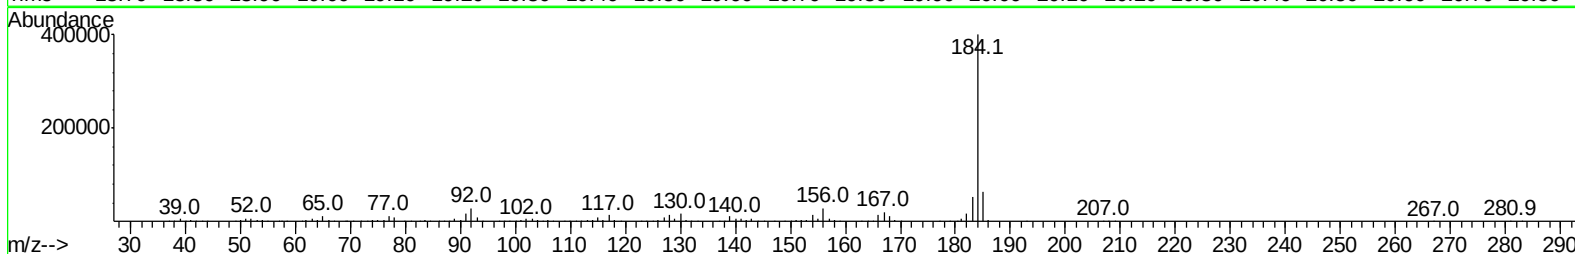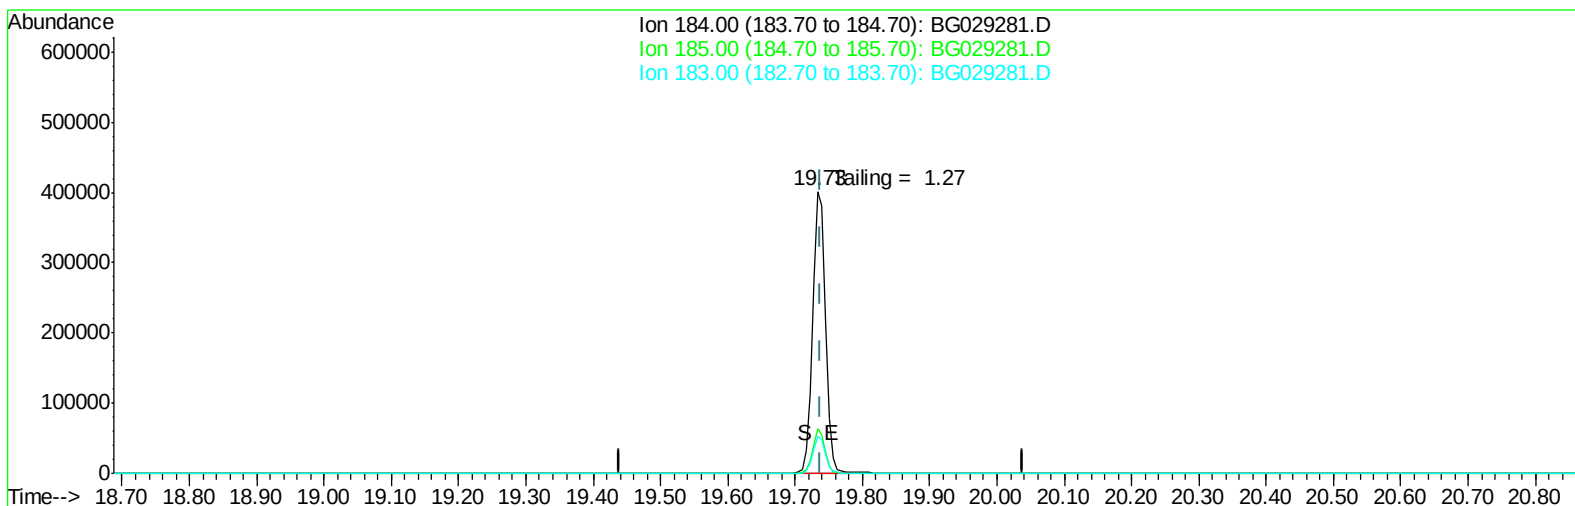

TIC: BG029281.D

(76) Benzidine

19.734min (-0.006) 313521.00ng

response 549047

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.75
183.00	13.30	13.16
0.00	0.00	0.00