


Data Path : Z:\HPCHEM1\BNA G\Data\BG101617\
Data File : BG029281.D
Acq On : 16 Oct 2017 21:28
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG101617.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 16 17:32:15 2017

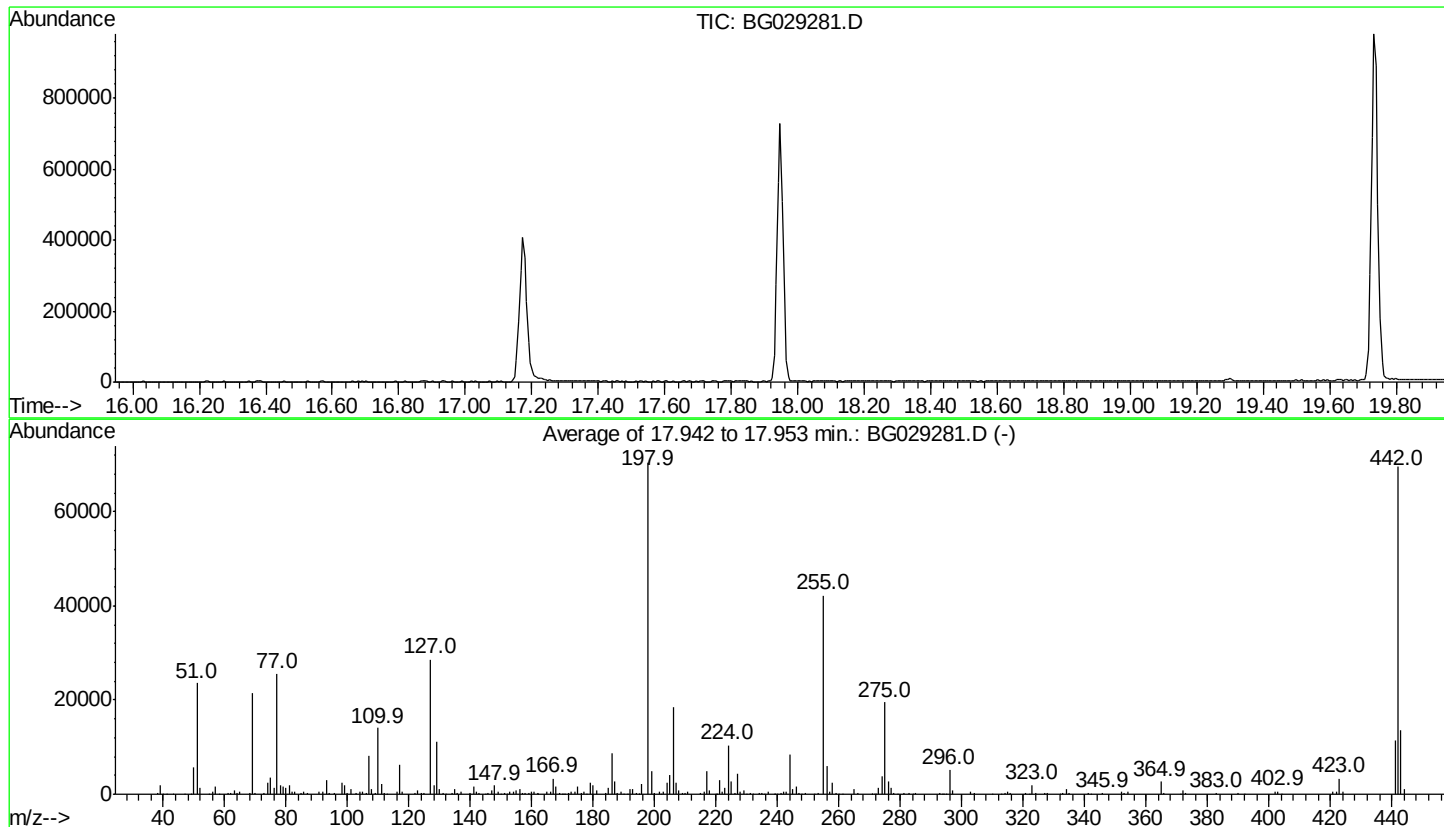

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	23538	PASS
68	69	0.00	2	1.1	227	PASS
69	198	0.00	100	30.4	21414	PASS
70	69	0.00	2	0.9	198	PASS
127	198	10	80	40.6	28578	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70440	PASS
199	198	5	9	6.9	4864	PASS
275	198	10	60	27.7	19509	PASS
365	198	1	100	3.8	2698	PASS
441	442	0.01	24	16.2	11322	PASS
442	198	50	100	99.0	69746	PASS
443	442	15	24	19.4	13563	PASS