
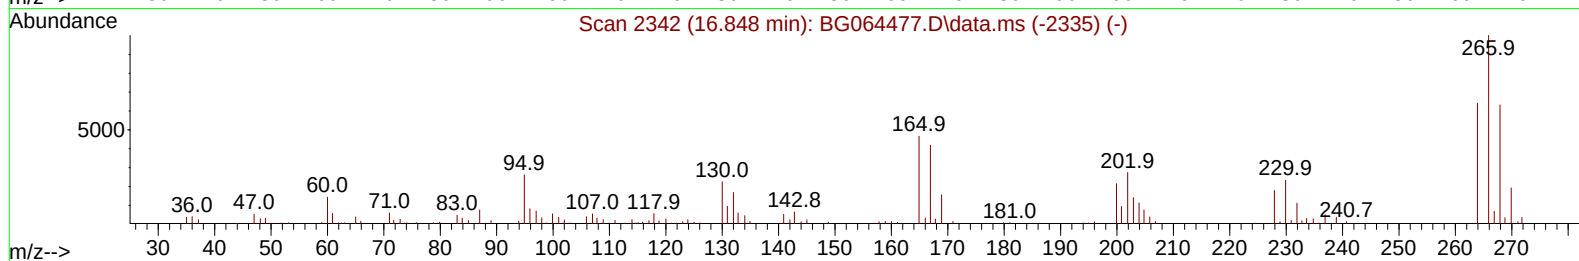
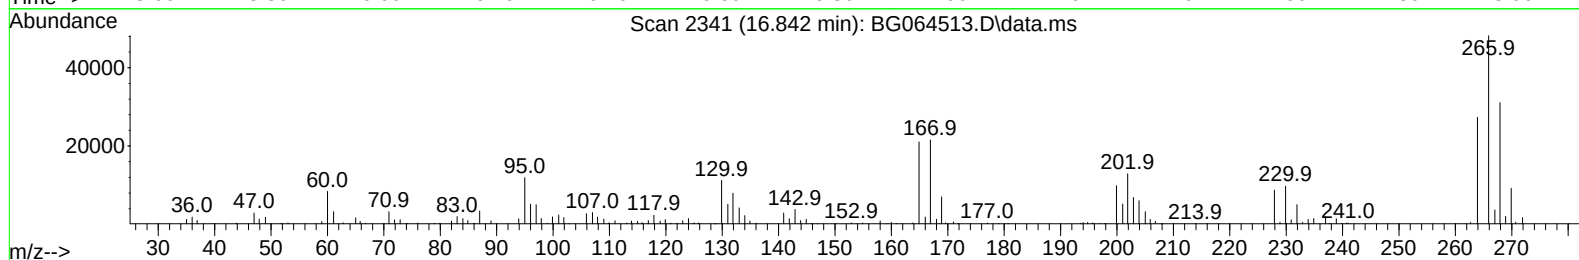


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101625\
Data File : BG064513.D
Acq On : 16 Oct 2025 12:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 16:24:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

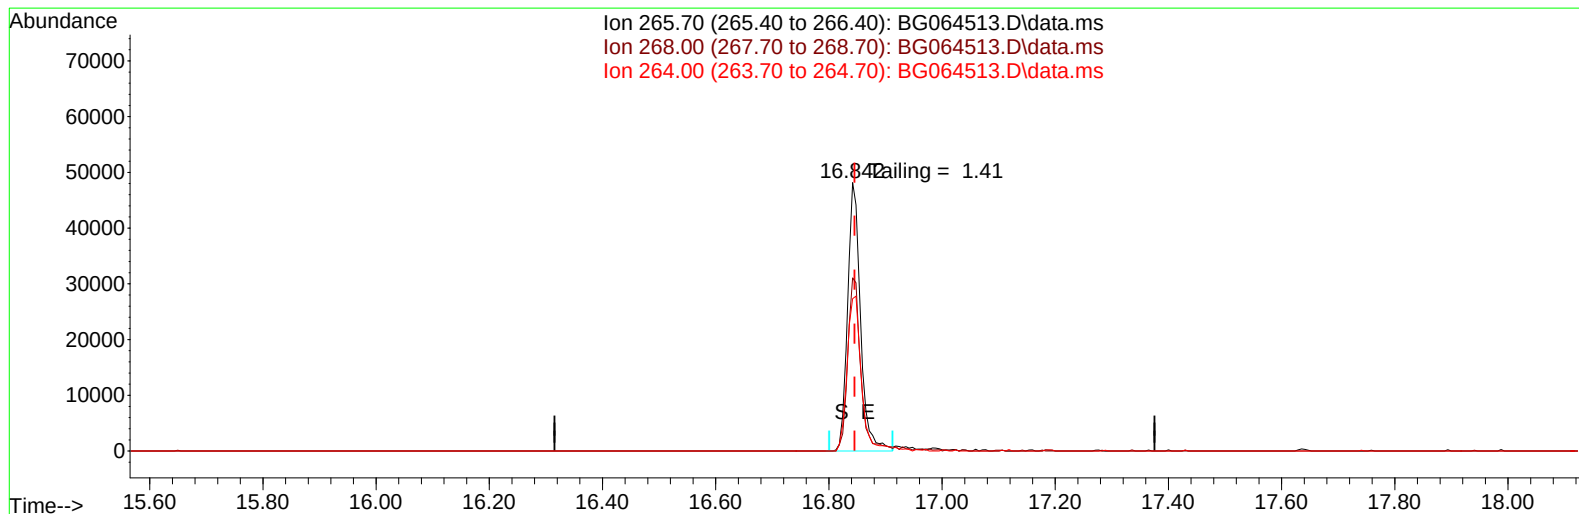

TIC: BG064513.D\data.ms

(70) Pentachlorophenol (C)




16.842min (-0.003) 173683.49 ng

response 76577

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	64.52
264.00	64.00	56.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101625\
Data File : BG064513.D
Acq On : 16 Oct 2025 12:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 16:24:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

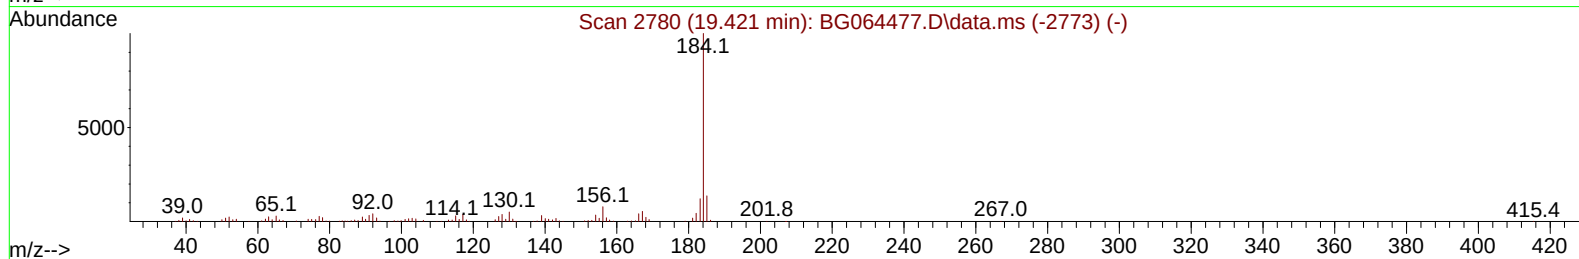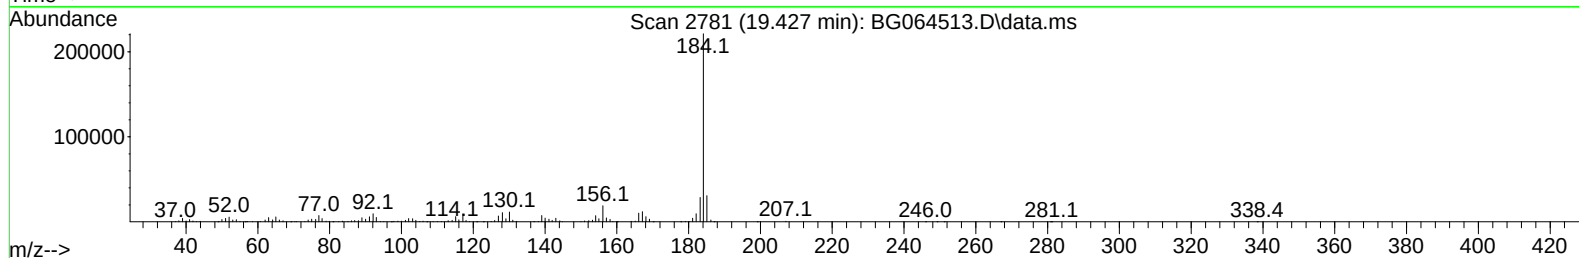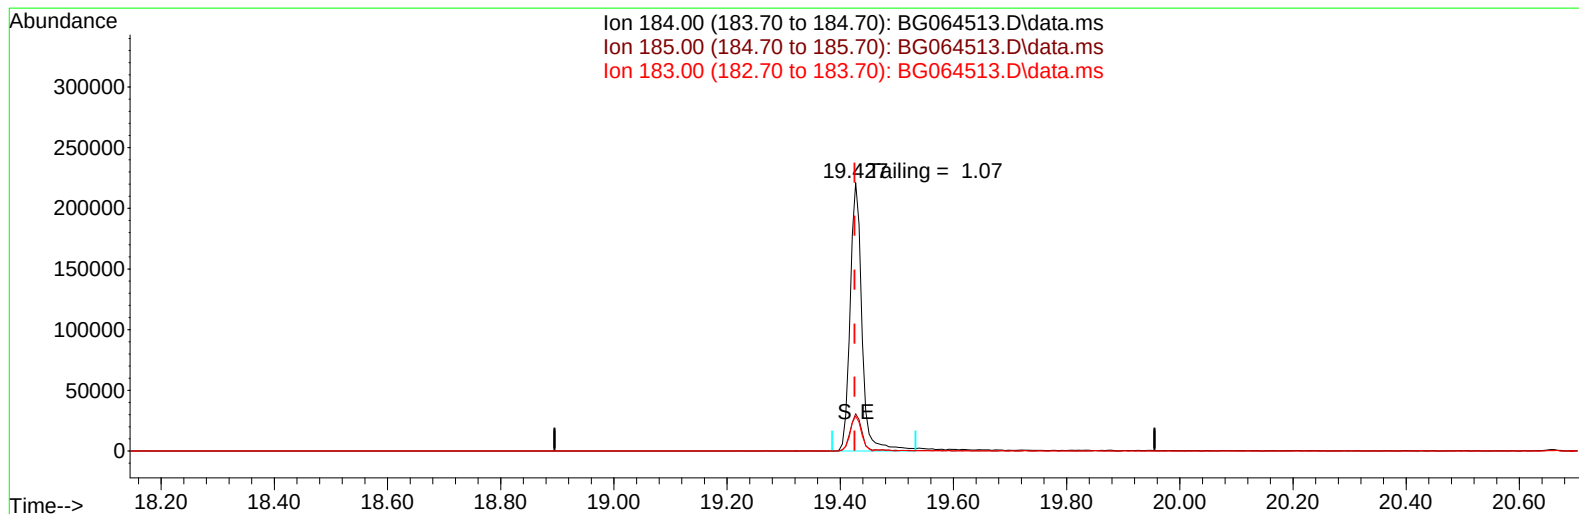

TIC: BG064513.D\data.ms

(77) Benzidine**19.427min (+ 0.002) 225557.91 ng****response 319923**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.91
183.00	12.20	13.03
0.00	0.00	0.00