


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101625\
Data File : BG064513.D
Acq On : 16 Oct 2025 12:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 02 16:40:42 2025

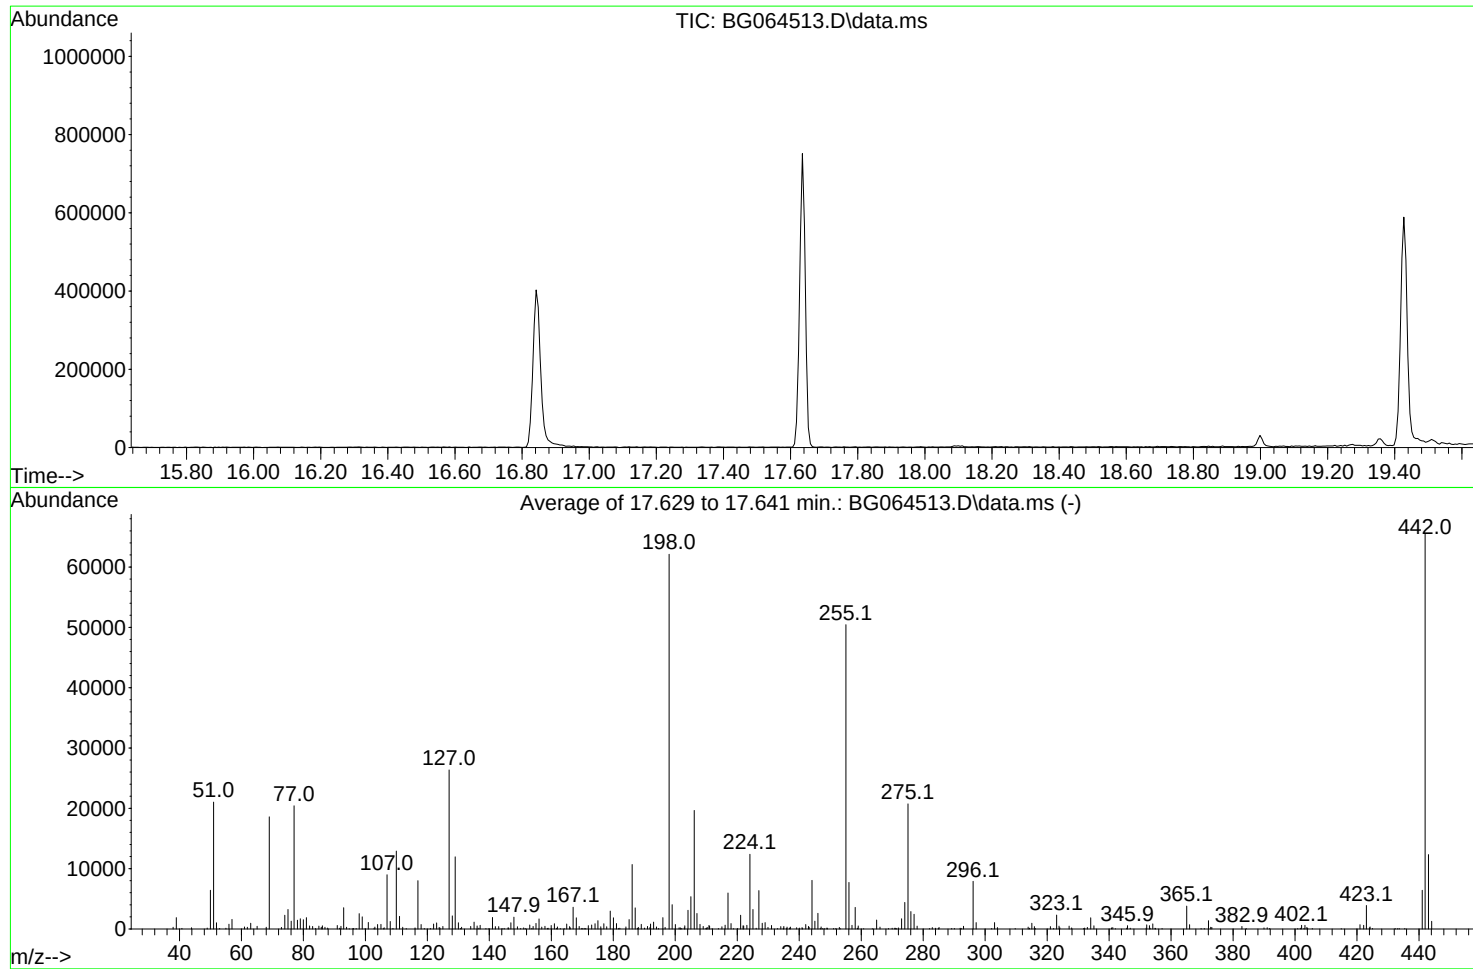




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.5	281	PASS
69	69	100	100	100.0	18586	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.4	244	PASS
198	198	100	100	100.0	62131	PASS
199	198	5	9	6.5	4017	PASS
365	198	1	100	6.1	3782	PASS
441	443	0.01	150	52.1	6421	PASS
442	442	100	100	100.0	65464	PASS
443	442	15	24	18.8	12316	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101625\
Data File : BG064513.D
Acq On : 16 Oct 2025 12:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 16 16:24:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

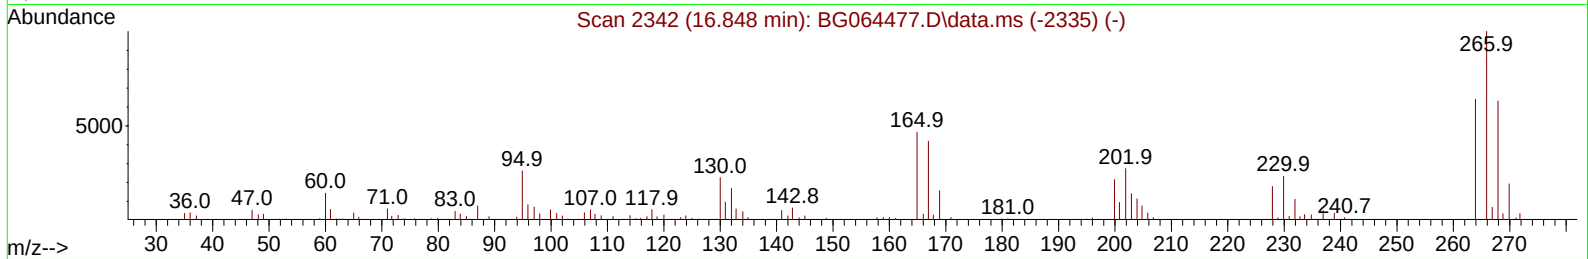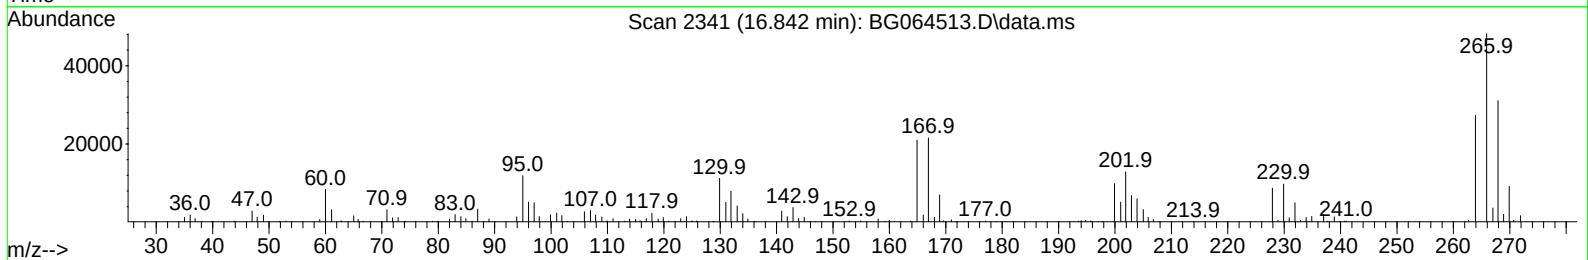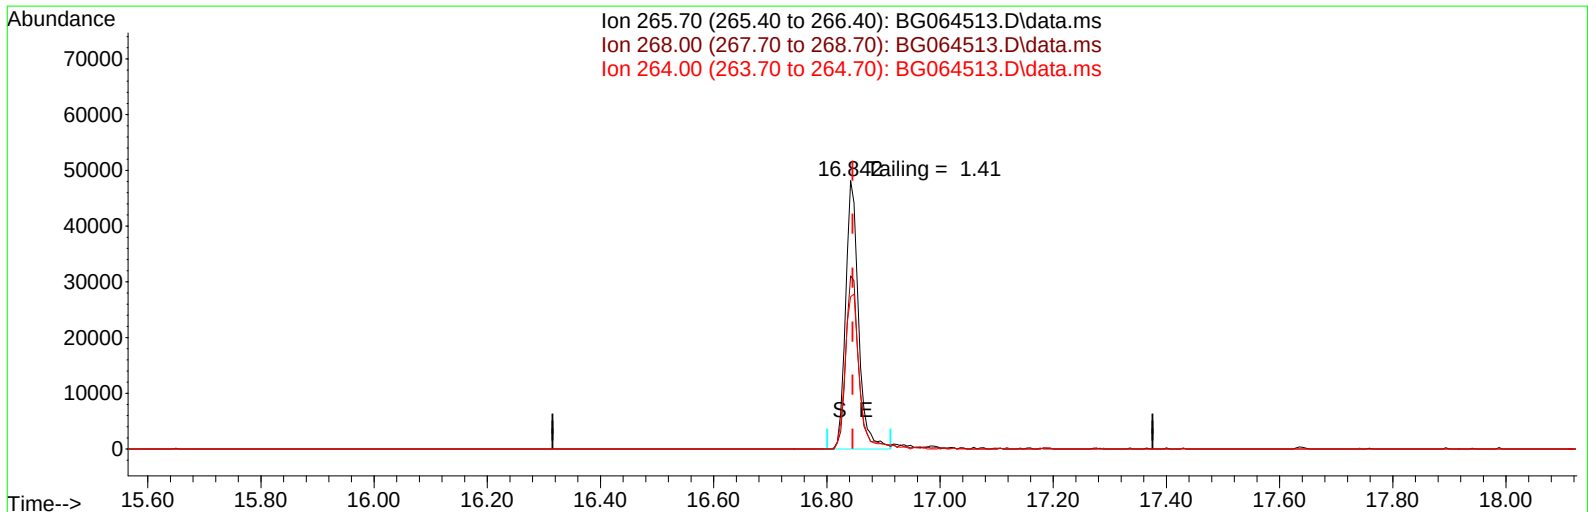

TIC: BG064513.D\data.ms

(70) Pentachlorophenol (C)

16.842min (-0.003) 173683.49 ng




response 76577

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	64.52
264.00	64.00	56.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101625\
Data File : BG064513.D
Acq On : 16 Oct 2025 12:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 16 16:24:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

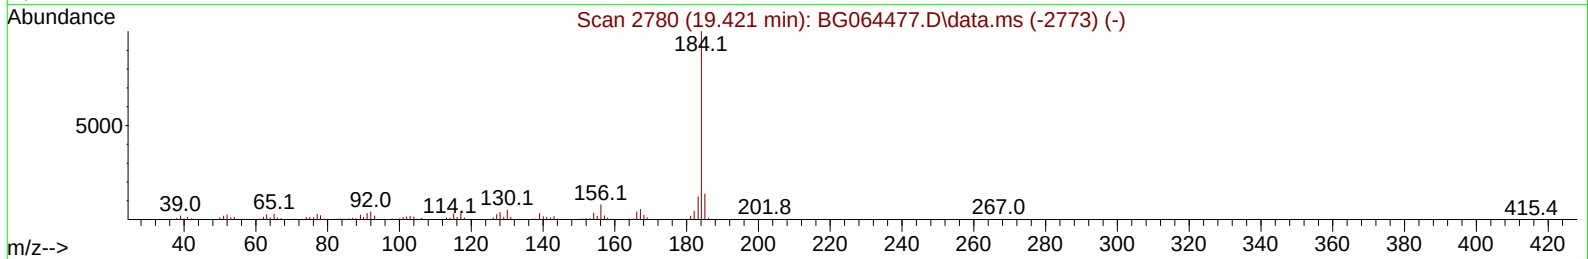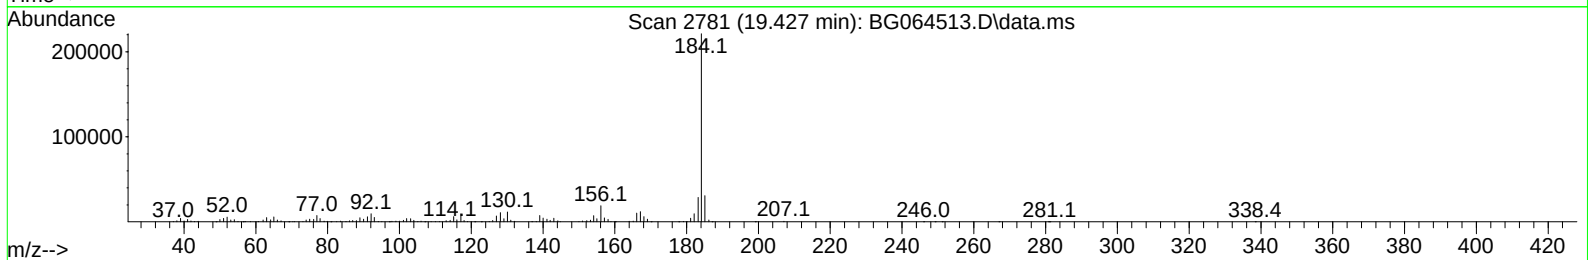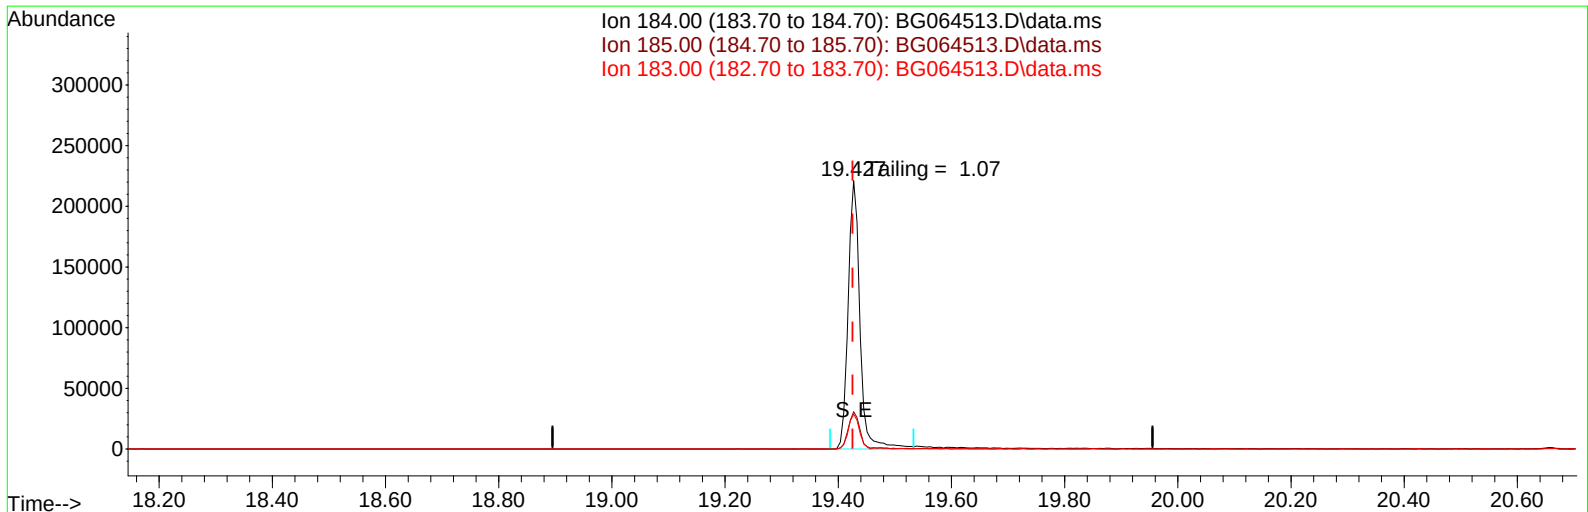

TIC: BG064513.D\data.ms

(77) Benzidine

19.427min (+ 0.002) 225557.91 ng

response 319923

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.91
183.00	12.20	13.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/16/2025	BNA_G	<u>BG064513.D</u>
Compound Name	Response	Retention Time
DDT	231734	20.655
DDD	2870	20.22
DDE	458	19.715
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3328	235062	1.42

Instrument :
BNA_G
ClientSampleId :
DFTPP