

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101716\
 Data File : BG024383.D
 Acq On : 17 Oct 2016 15:08
 Operator : UM/SJ
 Sample : H5239-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC751

Quant Time: Oct 17 15:41:57 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 15 05:09:35 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.28	152	149869	20.00	ng/ul	0.00
18) Naphthalene-d8	11.11	136	695199	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.90	164	594708	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.64	188	1263610	20.00	ng/ul	0.00
75) Chrysene-d12	21.94	240	1398271	20.00	ng/ul	0.00
83) Perylene-d12	25.38	264	1431209	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.64	96	2140	0.68	ng/uL	0.00
5) Phenol-d5	7.41	99	63613	4.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.60	67	136915	14.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.81	132	130142	13.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.97	113	115311	10.20	ng/ul	0.00
19) Nitrobenzene-d5	9.46	128	84817	17.19	ng/ul	0.00
22) 2-Nitrophenol-d4	10.19	143	95330	17.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.72	165	180217	14.99	ng/ul	0.00
29) 4-Chloroaniline-d4	11.25	131	4485	0.36	ng/ul	0.00
43) Dimethylphthalate-d6	14.29	166	708877	17.07	ng/ul	0.00
46) Acenaphthylene-d8	14.59	160	805883	16.94	ng/ul	0.00
51) 4-Nitrophenol-d4	15.06	143	32227	4.38	ng/ul	0.00
57) Fluorene-d10	15.89	176	657282	16.74	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.99	200	116064	15.28	ng/ul	0.00
70) Anthracene-d10	17.74	188	994924	17.43	ng/ul	0.00
76) Pyrene-d10	20.01	212	1148883	17.60	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.14	264	1113721	17.30	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.34	163	43201	1.06	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101716\
Data File : BG024383.D
Acq On : 17 Oct 2016 15:08
Operator : UM/SJ
Sample : H5239-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BC751

Quant Time: Oct 17 15:41:57 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 15 05:09:35 2016
Response via : Initial Calibration

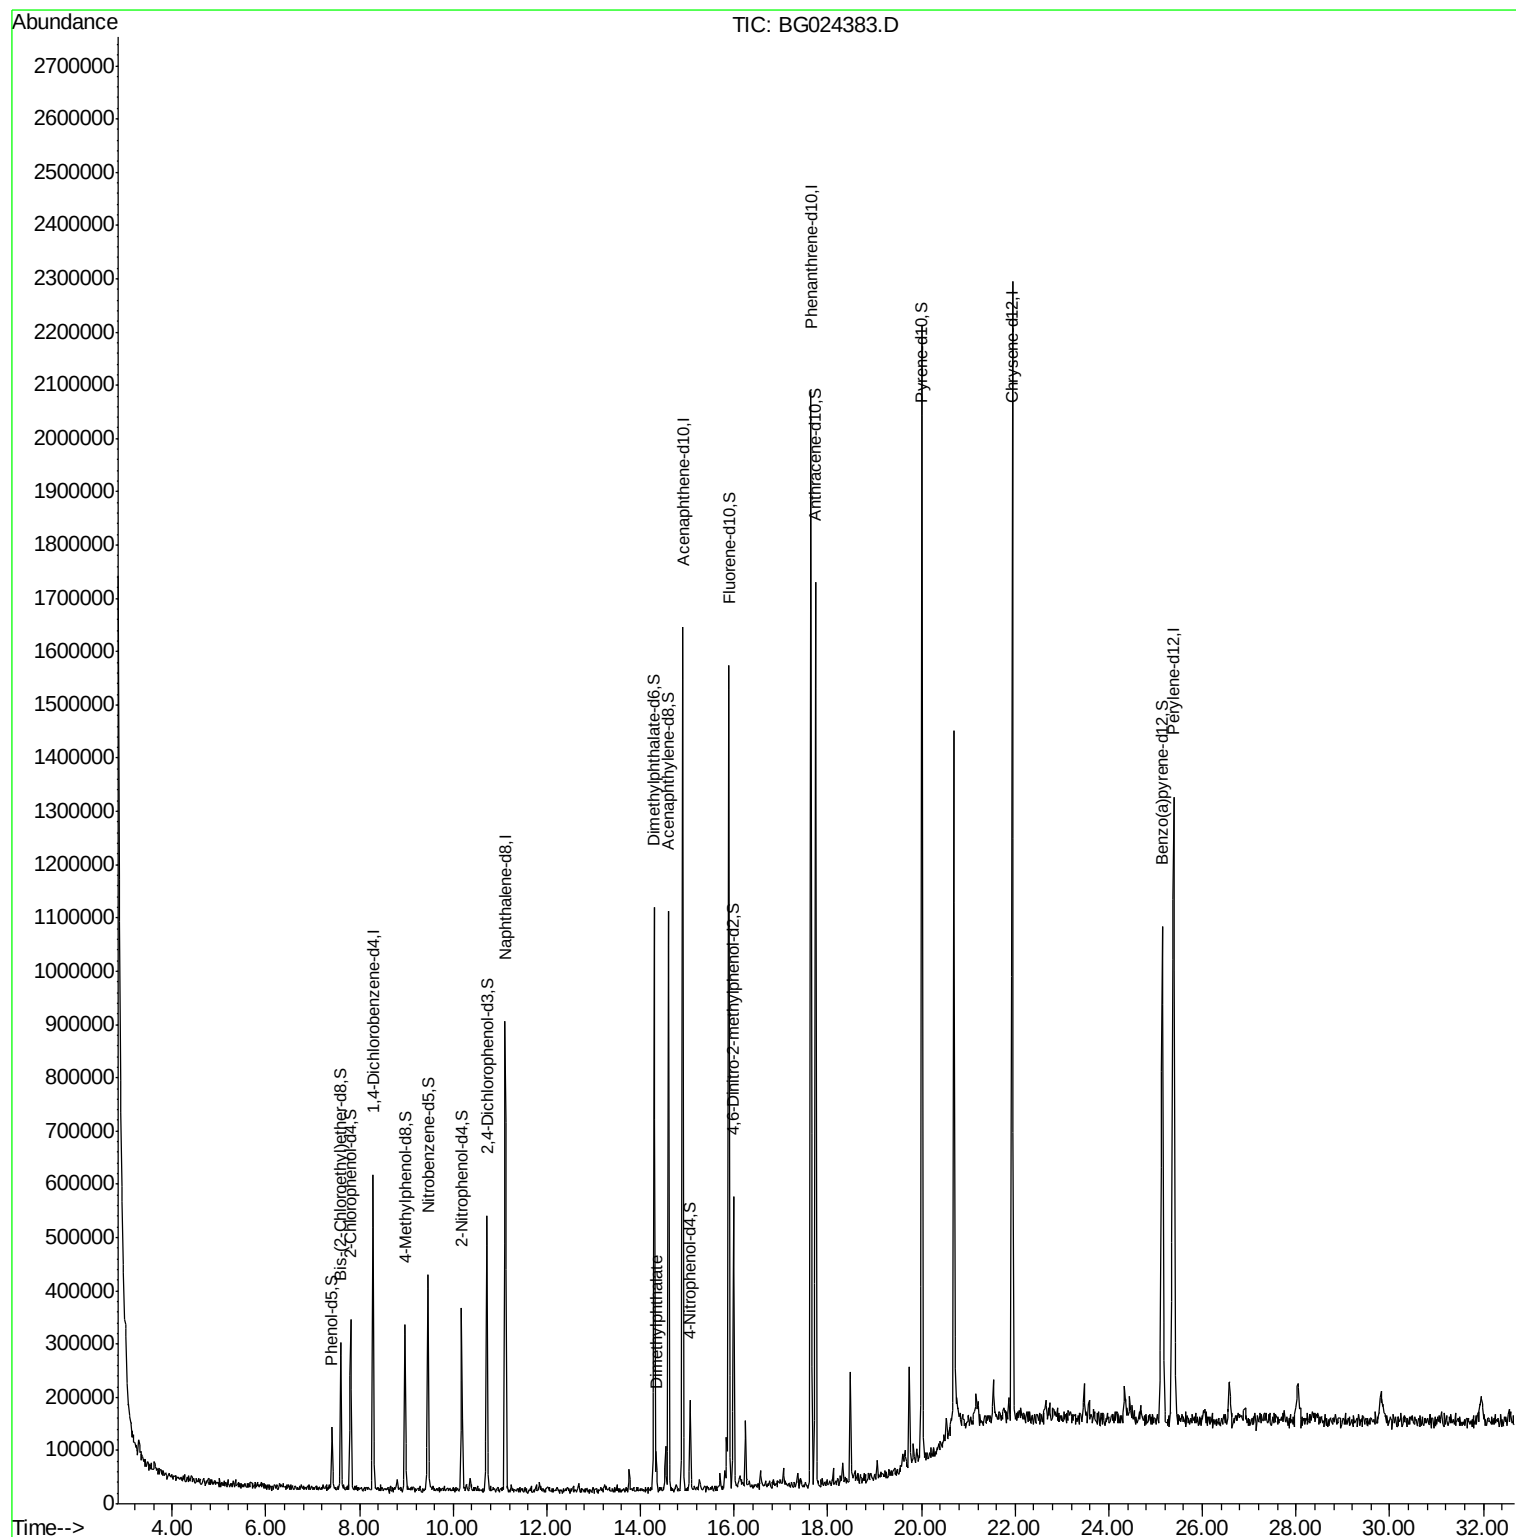

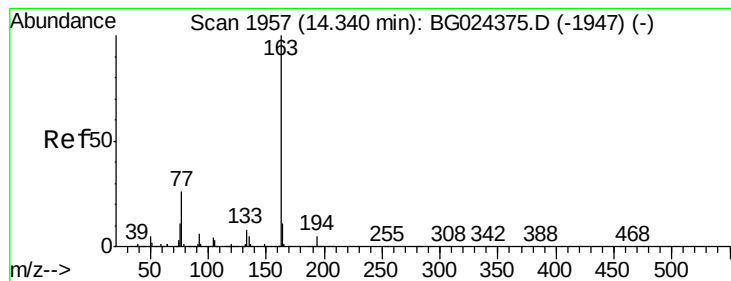

#44

Dimethylphthalate

Concen: 1.06 ng/ul

RT: 14.34 min Scan# 1957

Delta R.T. -0.00 min

Lab File: BG024383.D

Acq: 17 Oct 2016 15:08

Instrument :

BNA_G

ClientSampleId :

BC751


Tot Ion:163 Resp: 43201

Ion Ratio Lower Upper

163 100

194 2.4 3.4 5.0#

164 8.2 9.0 13.4#

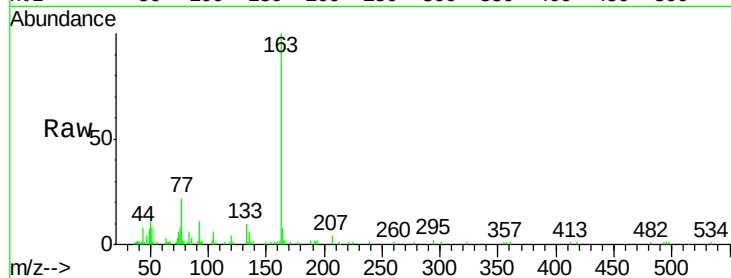

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

