

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101716\
 Data File : BG024392.D
 Acq On : 17 Oct 2016 20:54
 Operator : UM/SJ
 Sample : H5240-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDPF6

Manual Integrations
 APPROVED

umangi
 10/18/2016 6:10:57 PM

Quant Time: Oct 18 03:13:48 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 15 05:09:35 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.28	152	168694	20.00	ng/ul	0.00
18) Naphthalene-d8	11.12	136	837835	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.90	164	718581	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.64	188	1526747	20.00	ng/ul	0.00
75) Chrysene-d12	21.94	240	1723659	20.00	ng/ul	0.00
83) Perylene-d12	25.38	264	1746288	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.64	96	12560	3.54	ng/uL	0.00
5) Phenol-d5	7.41	99	292326	18.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.60	67	195226	18.35	ng/ul	0.00
9) 2-Chlorophenol-d4	7.81	132	207864	19.18	ng/ul	0.00
13) 4-Methylphenol-d8	8.97	113	250451	19.68	ng/ul	0.00
19) Nitrobenzene-d5	9.46	128	119386	20.08	ng/ul	0.00
22) 2-Nitrophenol-d4	10.18	143	135526	20.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.72	165	251730m	17.37	ng/ul	0.00
29) 4-Chloroaniline-d4	11.24	131	337386	22.16	ng/ul	0.00
43) Dimethylphthalate-d6	14.29	166	982843	19.59	ng/ul	0.00
46) Acenaphthylene-d8	14.59	160	1132029	19.70	ng/ul	0.00
51) 4-Nitrophenol-d4	15.06	143	146004	16.41	ng/ul	0.00
57) Fluorene-d10	15.88	176	922285	19.44	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.99	200	157498	17.17	ng/ul	0.00
70) Anthracene-d10	17.74	188	1396057	20.24	ng/ul	0.00
76) Pyrene-d10	20.01	212	1612912	20.05	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.14	264	1659608	21.12	ng/ul	0.00

Target Compounds

						Ovalue
6) Phenol	7.44	94	24153	1.51	ng/ul	93
44) Dimethylphthalate	14.34	163	464603	9.44	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG101716\
Data File : BG024392.D
Acq On : 17 Oct 2016 20:54
Operator : UM/SJ
Sample : H5240-04
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BDPF6

Manual Integrations
APPROVED

umangi
10/18/2016 6:10:57 PM

Quant Time: Oct 18 03:13:48 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 15 05:09:35 2016
Response via : Initial Calibration

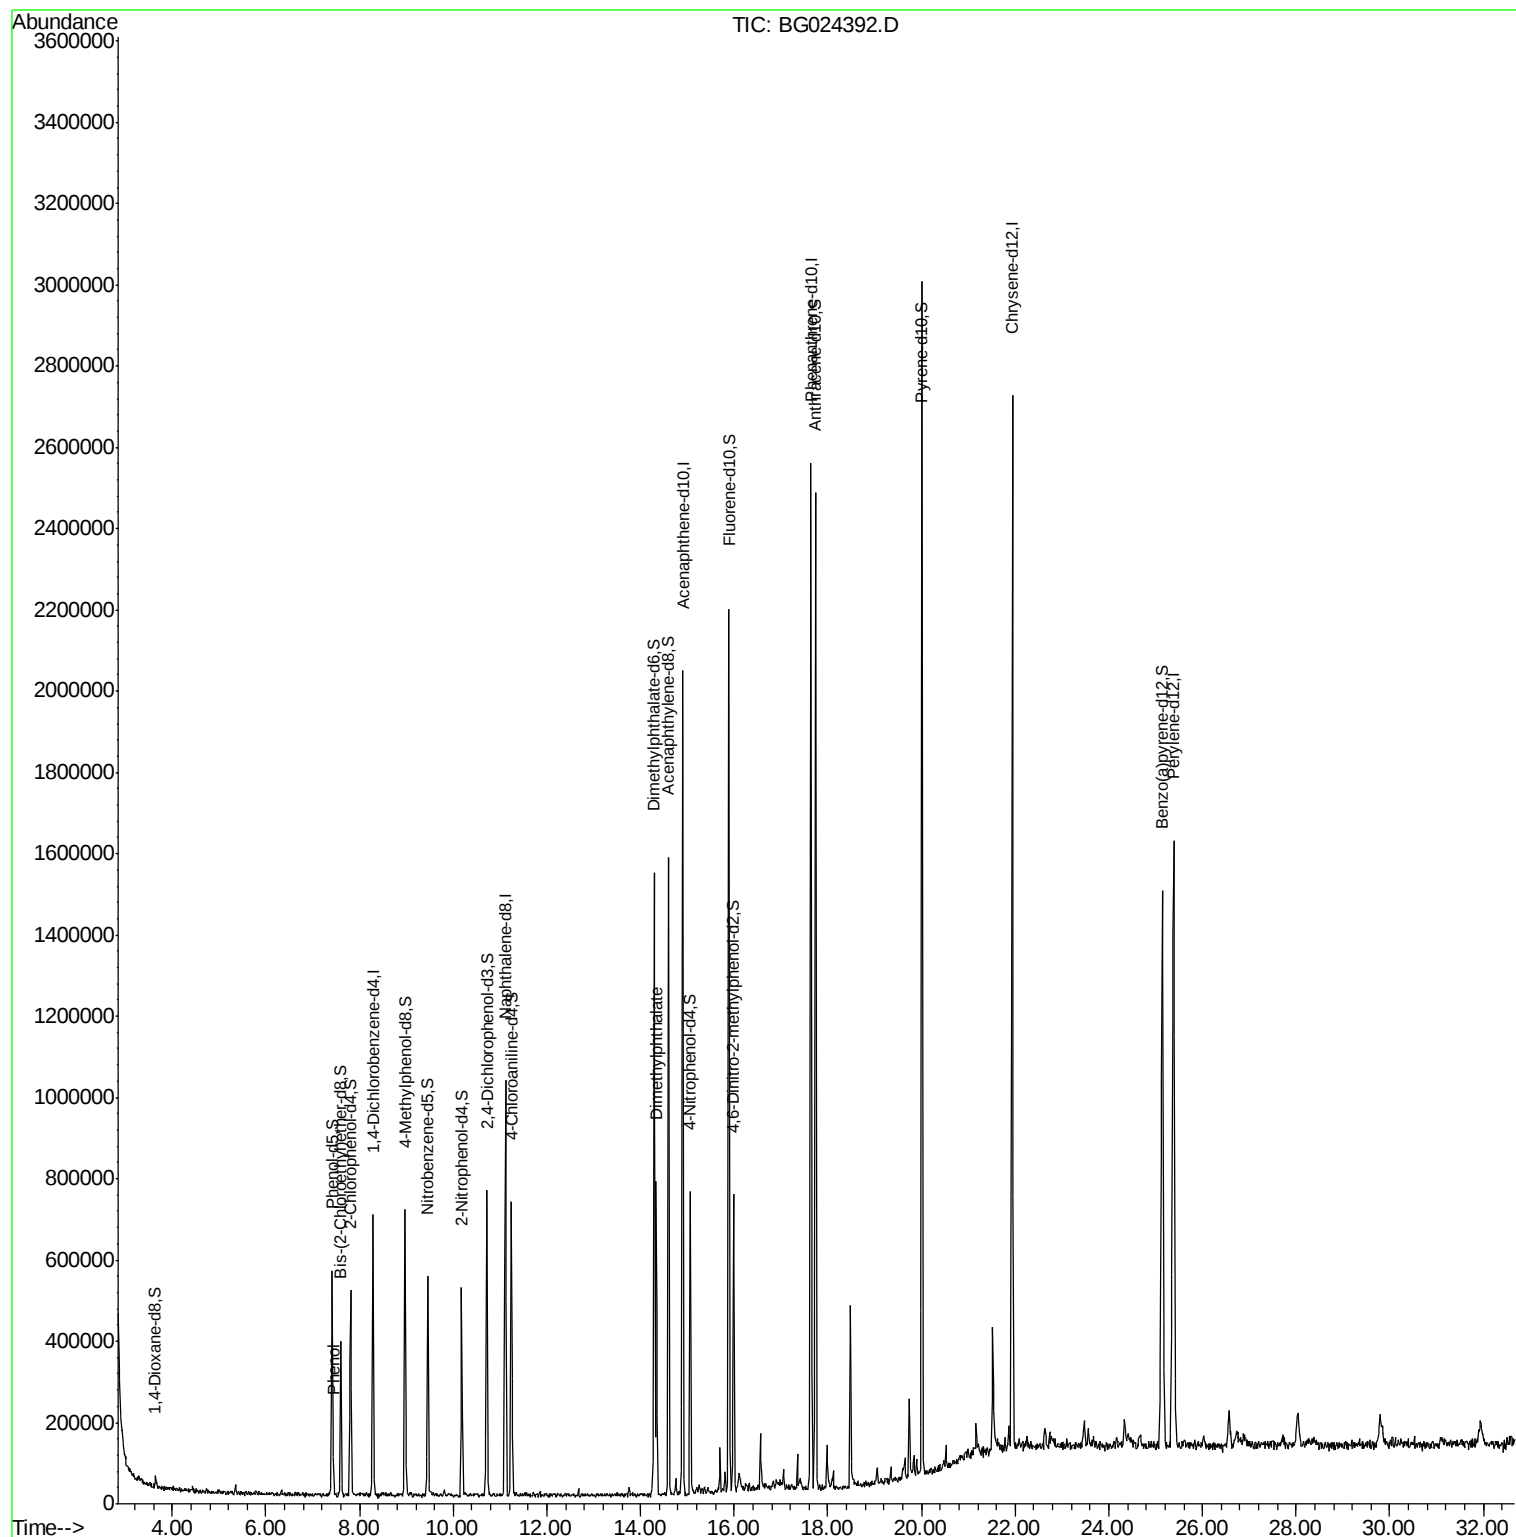

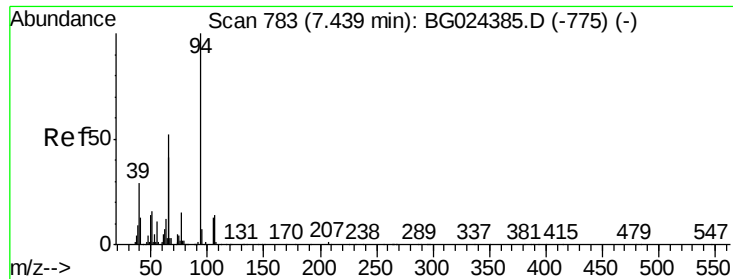

#6

Phenol

Concen: 1.51 ng/ul

RT: 7.44 min Scan# 784

Delta R.T. 0.00 min

Lab File: BG024392.D

Acq: 17 Oct 2016 20:54

Instrument :

BNA_G





ClientSampleId :

BDPF6

Tot Ion:	94	Resp:	24153
Ion	Ratio	Lower	Upper
94	100		
65	30.8	26.8	40.2
66	49.5	44.4	66.6

Manual Integrations
APPROVED

umangi
10/18/2016 6:10:57 PM

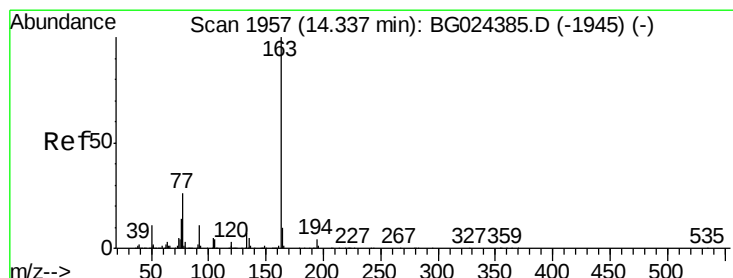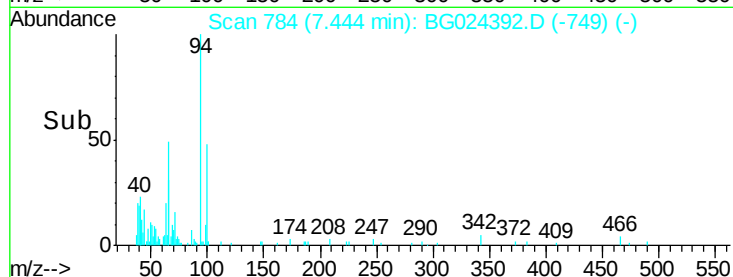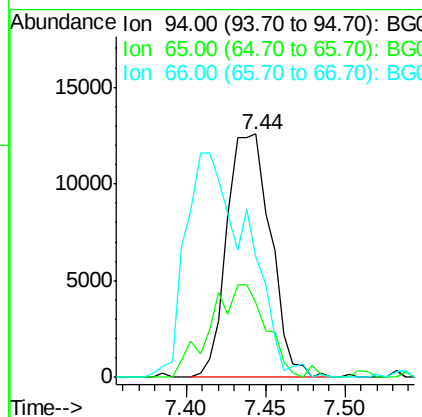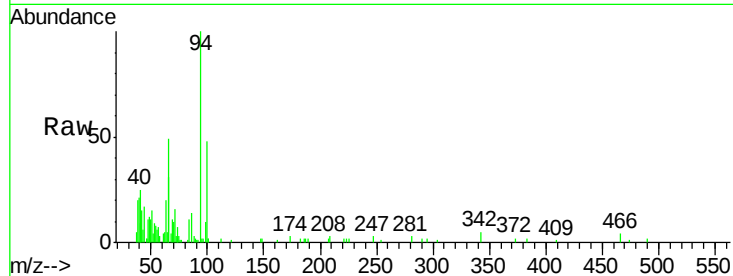

#44

Dimethylphthalate

Concen: 9.44 ng/ul

RT: 14.34 min Scan# 1957

Delta R.T. -0.00 min

Lab File: BG024392.D

Acq: 17 Oct 2016 20:54

Tgt Ion:	163	Resp:	464603
Ion	Ratio	Lower	Upper
163	100		
194	4.9	3.4	5.0
164	10.4	9.0	13.4

