

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101716\
 Data File : BG024414.D
 Acq On : 18 Oct 2016 11:02
 Operator : UM/SJ
 Sample : H5223-10
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDNK0

Manual Integrations
 APPROVED

umangi
 10/18/2016 6:11:27 PM

Quant Time: Oct 18 11:47:20 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 18 03:43:57 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.28	152	221673	20.00	ng/ul	0.00
18) Naphthalene-d8	11.11	136	1035719	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.90	164	888681	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.64	188	1786565m	20.00	ng/ul	0.00
75) Chrysene-d12	21.94	240	2029275	20.00	ng/ul	0.00
83) Perylene-d12	25.38	264	2152464	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.64	96	16594	3.55	ng/uL	0.00
5) Phenol-d5	7.41	99	431226	20.85	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.60	67	274673	19.65	ng/ul	0.00
9) 2-Chlorophenol-d4	7.81	132	298255	20.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.97	113	373113	22.32	ng/ul	0.00
19) Nitrobenzene-d5	9.46	128	170232	23.16	ng/ul	0.00
22) 2-Nitrophenol-d4	10.19	143	197702	24.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.71	165	361924	20.21	ng/ul	0.00
29) 4-Chloroaniline-d4	11.24	131	477130	25.36	ng/ul	0.00
43) Dimethylphthalate-d6	14.29	166	1362319	21.96	ng/ul	0.00
46) Acenaphthylene-d8	14.59	160	1529449	21.52	ng/ul	0.00
51) 4-Nitrophenol-d4	15.06	143	241226	21.92	ng/ul	0.00
57) Fluorene-d10	15.89	176	1259823	21.47	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.99	200	269096m	25.06	ng/ul	0.00
70) Anthracene-d10	17.74	188	1866442	23.13	ng/ul	0.00
76) Pyrene-d10	20.01	212	2126551	22.45	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.14	264	2259797	23.33	ng/ul	0.00

Target Compounds						Ovalue
6) Phenol	7.44	94	26861	1.28	ng/ul	95
44) Dimethylphthalate	14.34	163	663661	10.91	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG101716\
Data File : BG024414.D
Acq On : 18 Oct 2016 11:02
Operator : UM/SJ
Sample : H5223-10
Misc :
ALS Vial : 39 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BDNK0

Manual Integrations
APPROVED

umangi
10/18/2016 6:11:27 PM

Quant Time: Oct 18 11:47:20 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 18 03:43:57 2016
Response via : Initial Calibration

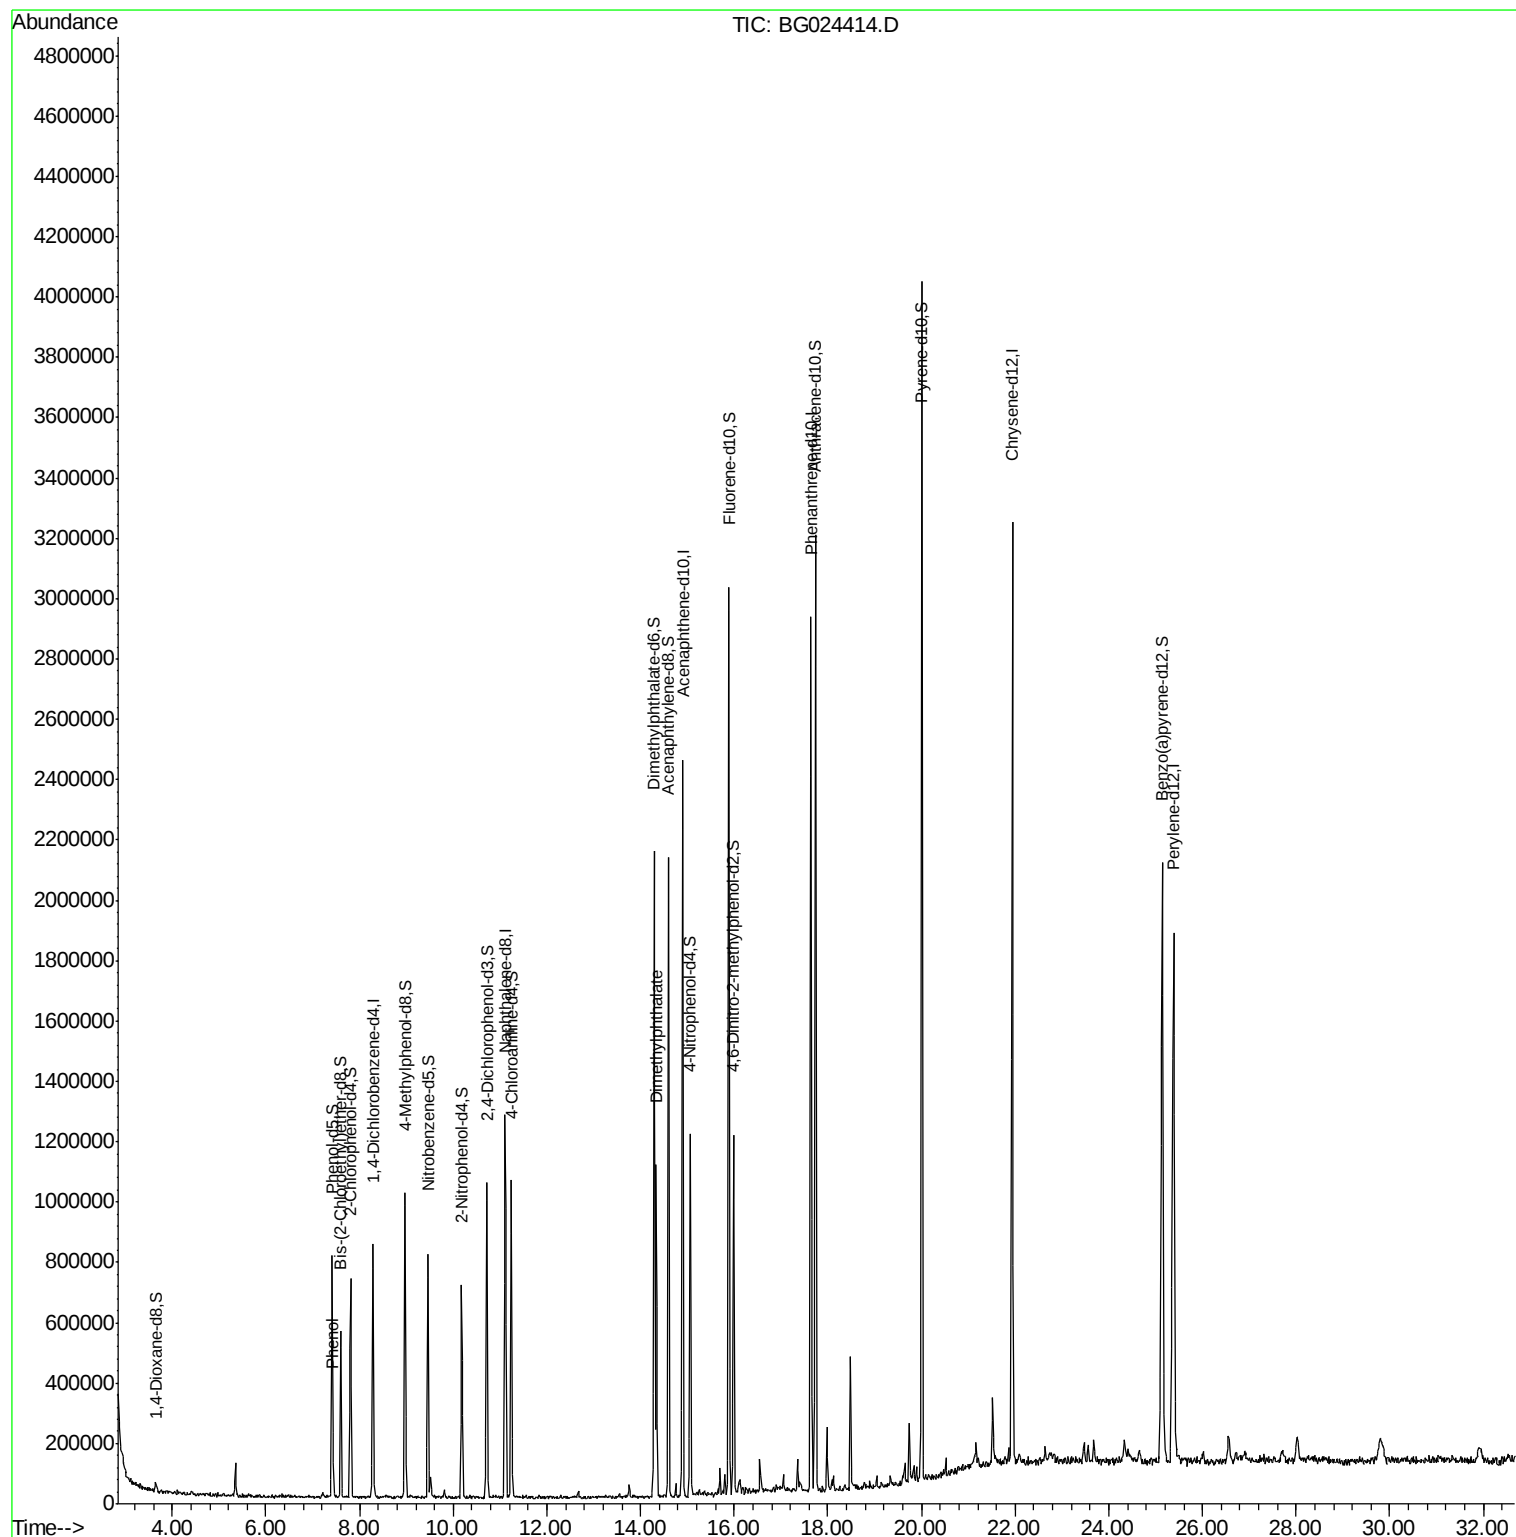

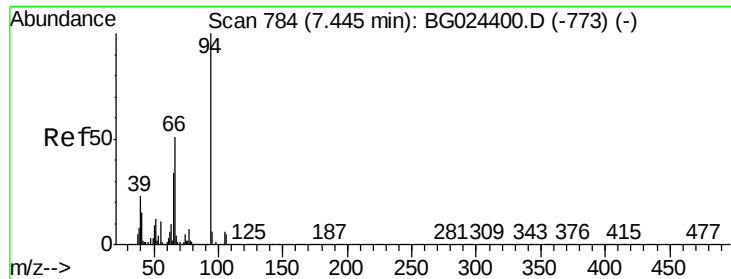

#6

Phenol

Concen: 1.28 ng/ul

RT: 7.44 min Scan# 783

Delta R.T. -0.01 min

Lab File: BG024414.D

Acq: 18 Oct 2016 11:02

Instrument :

BNA_G





ClientSampleId :

BDNK0

Tot Ion:	94	Resp:	26861
Ion Ratio	Lower	Upper	
94	100		
65	30.6	26.8	40.2
66	59.0	44.4	66.6

Manual Integrations
APPROVED

umangi
10/18/2016 6:11:27 PM

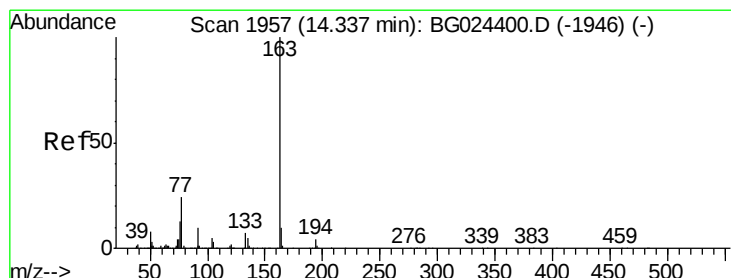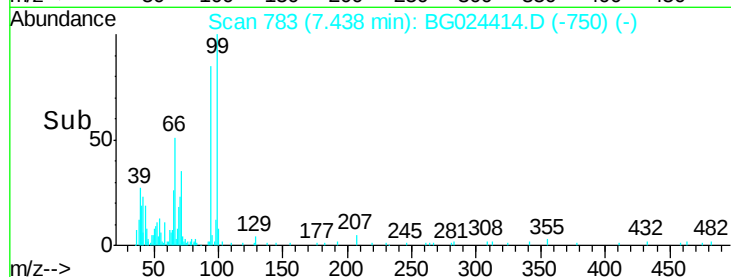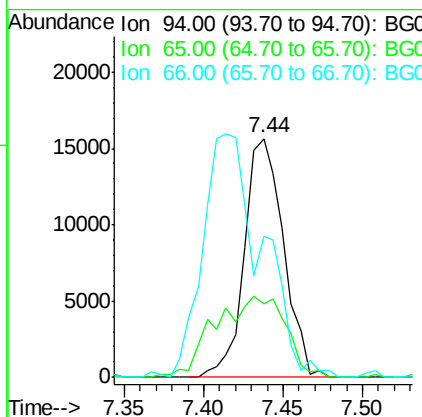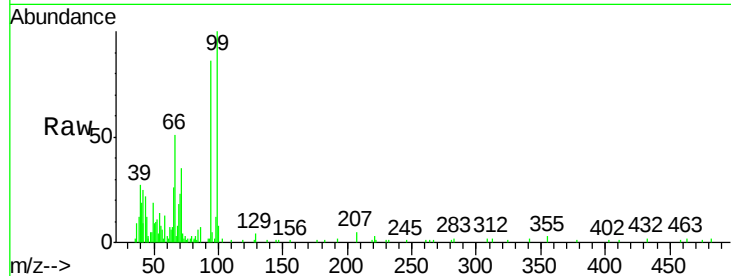

#44

Dimethylphthalate

Concen: 10.91 ng/ul

RT: 14.34 min Scan# 1957

Delta R.T. -0.00 min

Lab File: BG024414.D

Acq: 18 Oct 2016 11:02

Tgt Ion:	163	Resp:	663661
Ion Ratio	Lower	Upper	
163	100		
194	4.5	3.4	5.0
164	10.2	9.0	13.4

