

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101717\
 Data File : BG029314.D
 Acq On : 17 Oct 2017 23:30
 Operator : SJ/JU
 Sample : I5817-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Oct 18 00:56:25 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 16 17:32:15 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	69034	20.00	ng	0.00
21) Naphthalene-d8	10.98	136	342062	20.00	ng	0.00
38) Acenaphthene-d10	14.79	164	221670	20.00	ng	0.00
63) Phenanthrene-d10	17.52	188	500068	20.00	ng	0.00
75) Chrysene-d12	21.80	240	516800	20.00	ng	0.00
86) Perylene-d12	25.10	264	537897	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.72	112	206947	50.08	ng	0.00
7) Phenol-d6	7.32	99	185282	31.94	ng	0.00
23) Nitrobenzene-d5	9.33	82	533174	99.05	ng	0.00
41) 2,4,6-Tribromophenol	16.27	330	261640	91.42	ng	0.00
44) 2-Fluorobiphenyl	13.42	172	1387816	91.82	ng	0.00
78) Terphenyl-d14	20.11	244	1934641	85.16	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101717\
Data File : BG029314.D
Acq On : 17 Oct 2017 23:30
Operator : SJ/JU
Sample : I5817-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Oct 18 00:56:25 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 16 17:32:15 2017
Response via : Initial Calibration

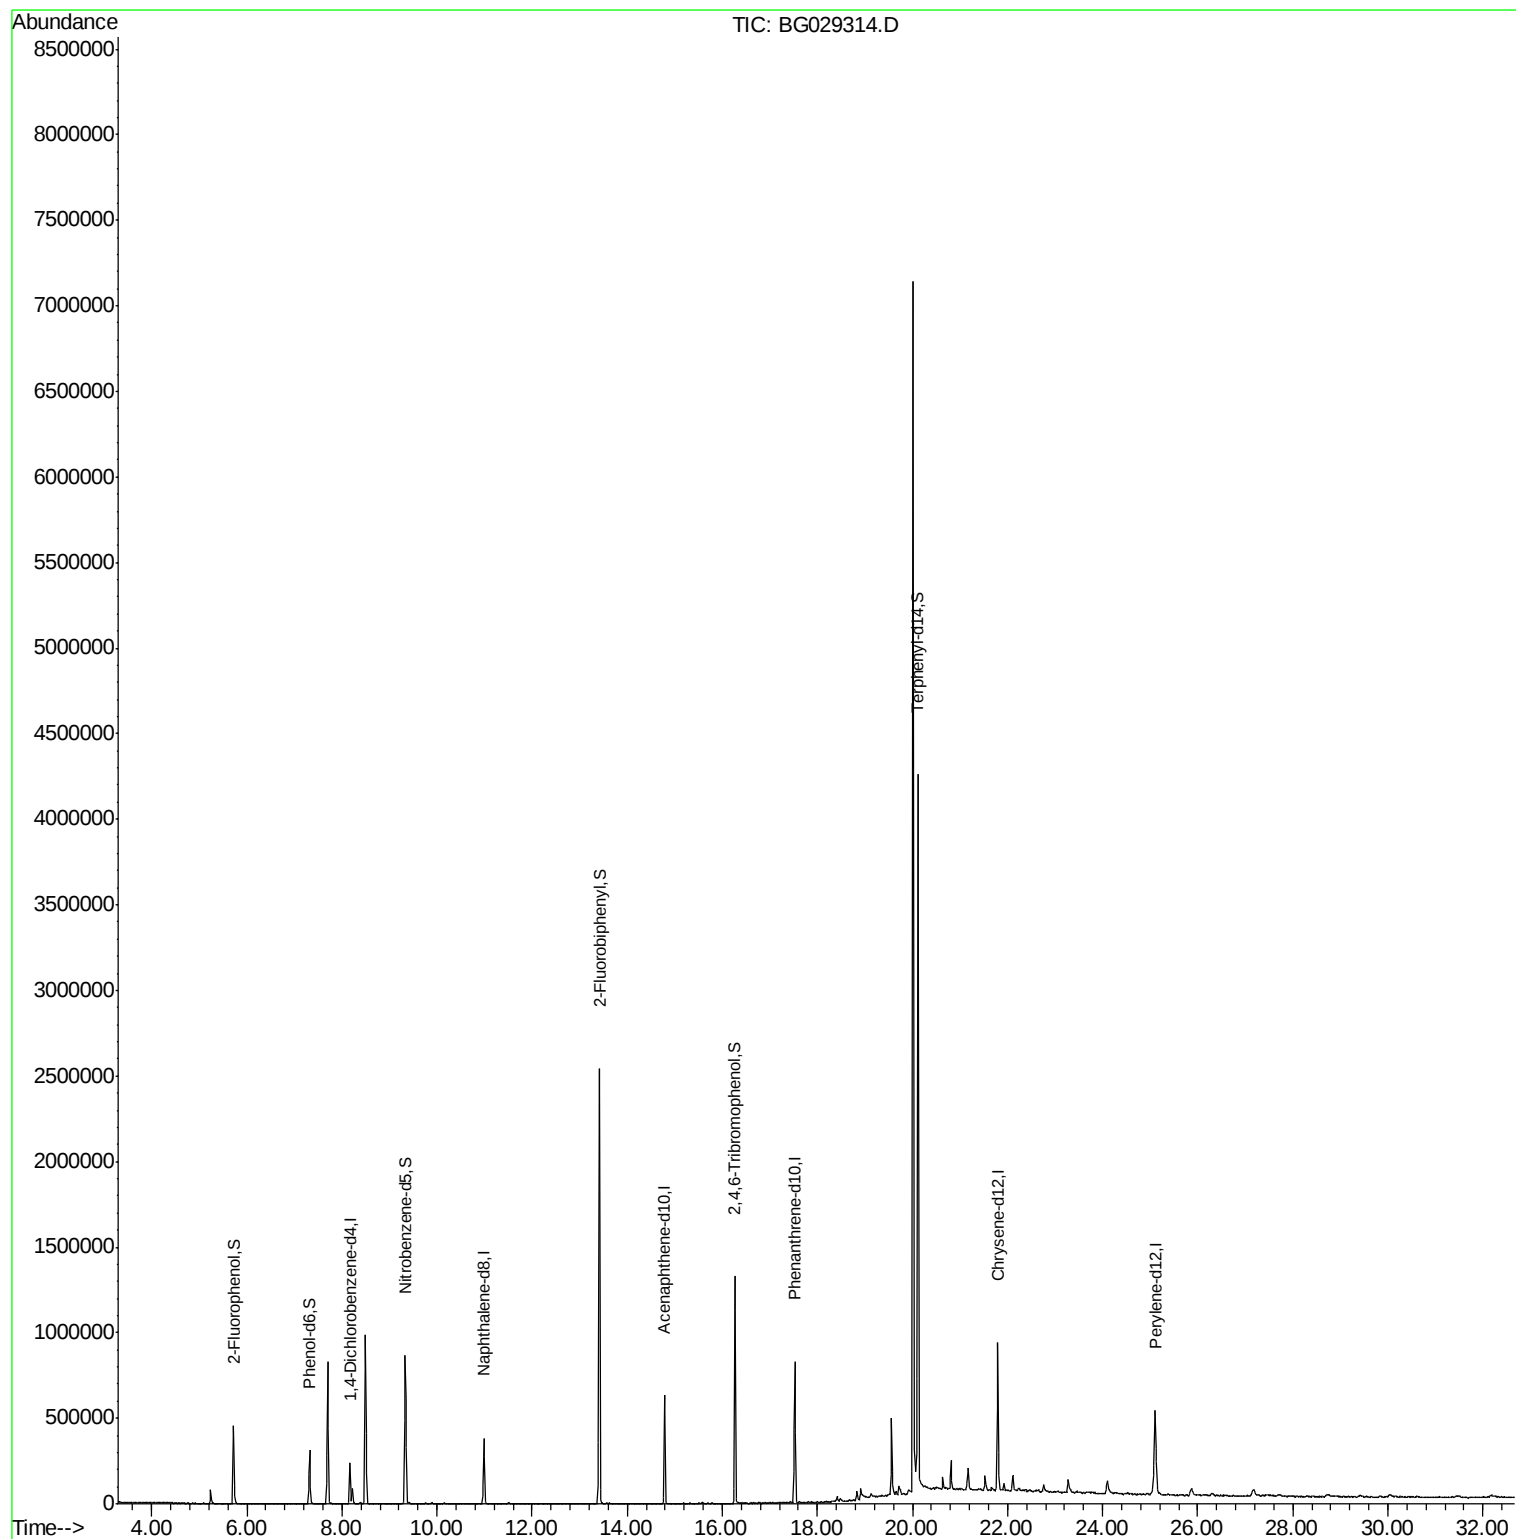

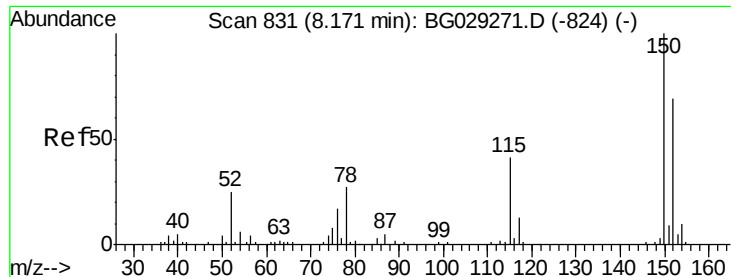


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.17 min Scan# 831
Delta R.T. -0.00 min
Lab File: BG029314.D
Acq: 17 Oct 2017 23:30

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 69034
Ion Ratio Lower Upper
152 100
150 159.9 126.6 189.8
115 55.4 53.0 79.4

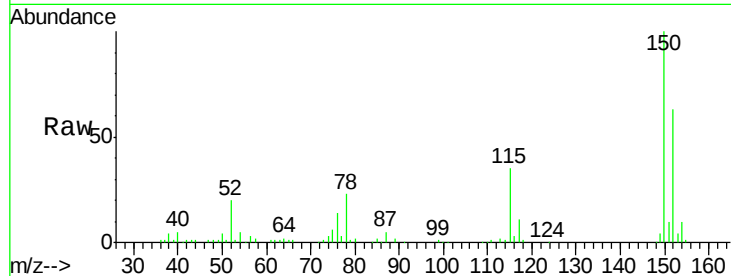


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

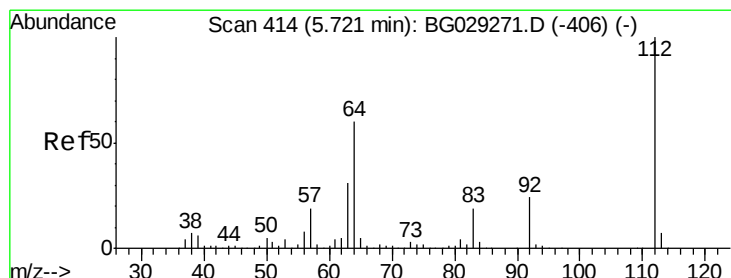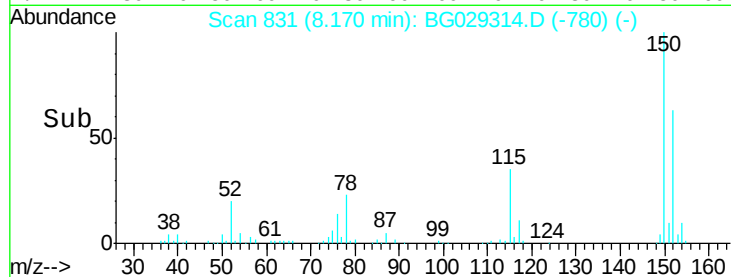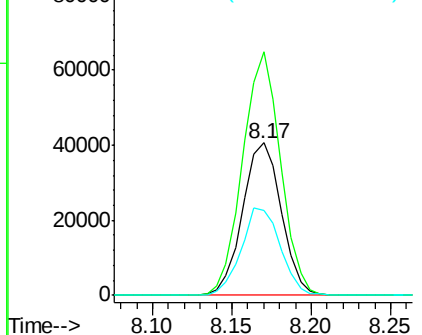



#5


2-Fluorophenol
Concen: 50.08 ng
RT: 5.72 min Scan# 414
Delta R.T. -0.00 min
Lab File: BG029314.D
Acq: 17 Oct 2017 23:30

Tgt Ion:112 Resp: 206947
Ion Ratio Lower Upper
112 100
64 60.3 56.3 84.5
63 31.3 30.1 45.1

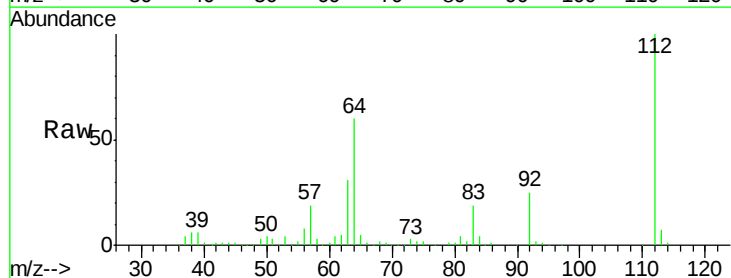

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

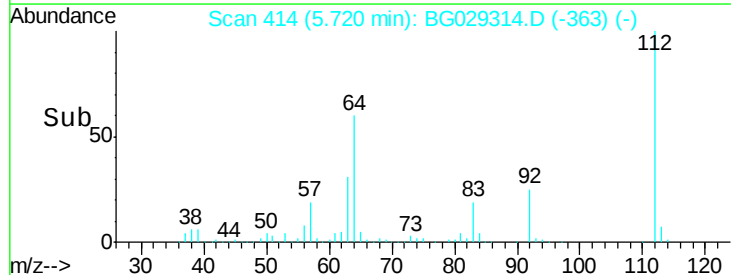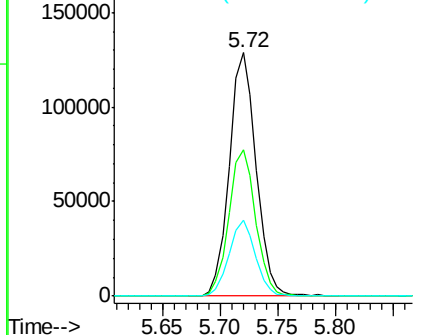

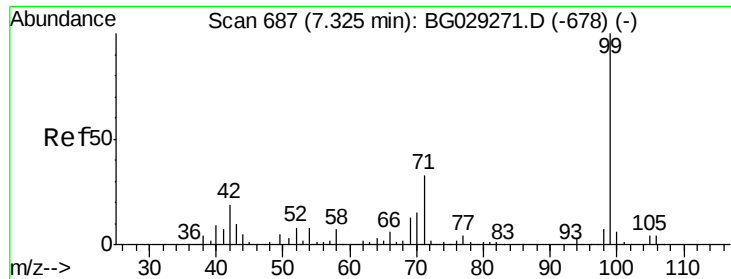

#7

Phenol-d6

Concen: 31.94 ng

RT: 7.32 min Scan# 686

Delta R.T. -0.01 min

Lab File: BG029314.D

Acq: 17 Oct 2017 23:30

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 185282

Ion Ratio Lower Upper




99 100

42 19.3 14.1 21.1

71 32.2 26.1 39.1

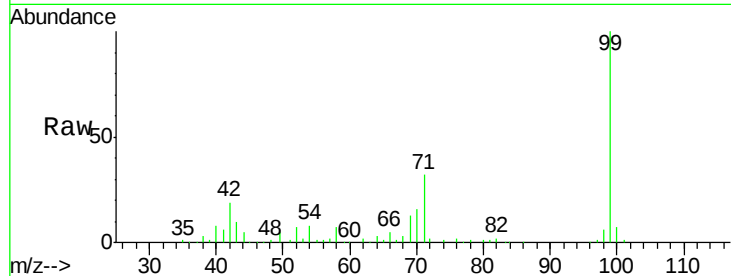

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

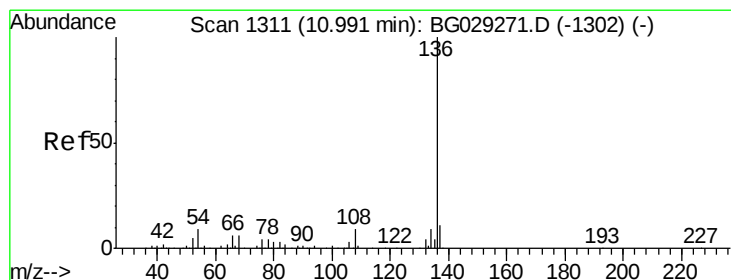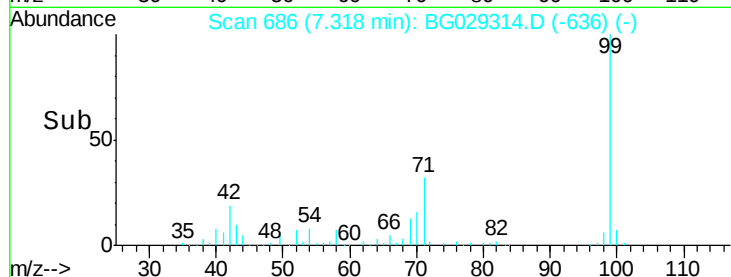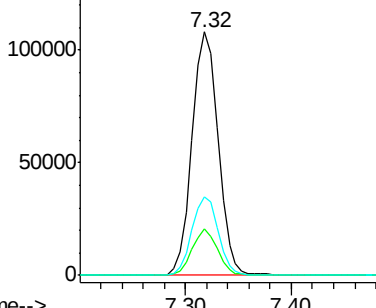

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.98 min Scan# 1310

Delta R.T. -0.01 min

Lab File: BG029314.D

Acq: 17 Oct 2017 23:30

Tgt Ion: 136 Resp: 342062


Ion Ratio Lower Upper

136 100



137 11.3 9.2 13.8


54 8.5 10.3 15.5#

68 6.0 4.5 6.7

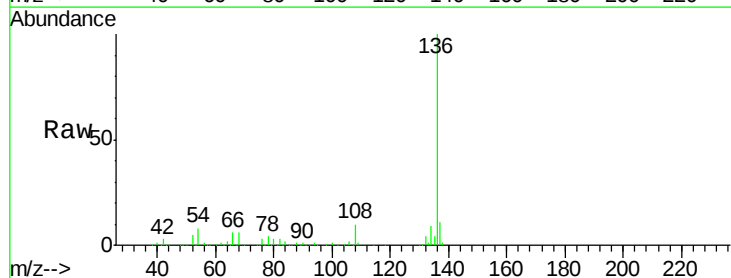

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



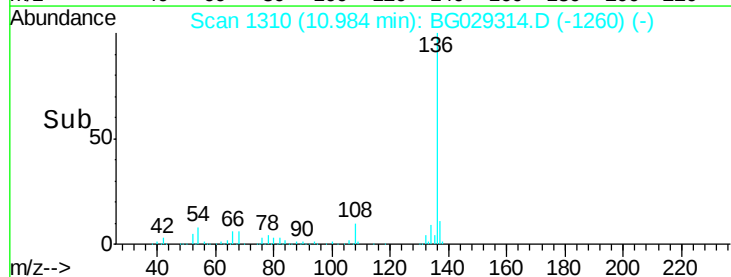
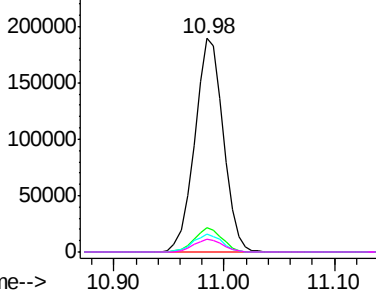


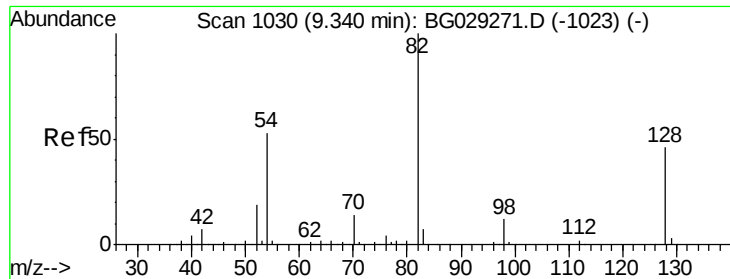

#23
 Nitrobenzene-d5
 Concen: 99.05 ng
 RT: 9.33 min Scan# 1029
 Delta R.T. -0.01 min
 Lab File: BG029314.D
 Acq: 17 Oct 2017 23:30




Instrument :
 BNA_G
 ClientSampled :


Tot Ion: 82 Resp: 533174
 Ion Ratio Lower Upper
 82 100
 128 45.0 29.7 44.5#
 54 52.3 43.1 64.7

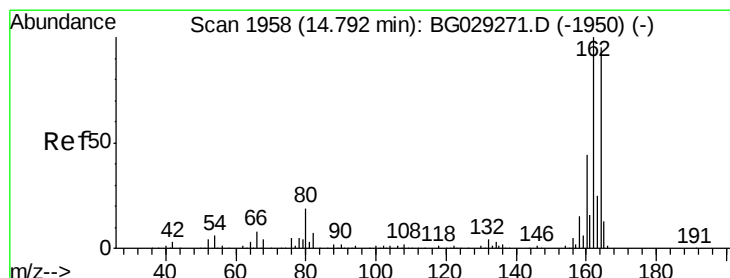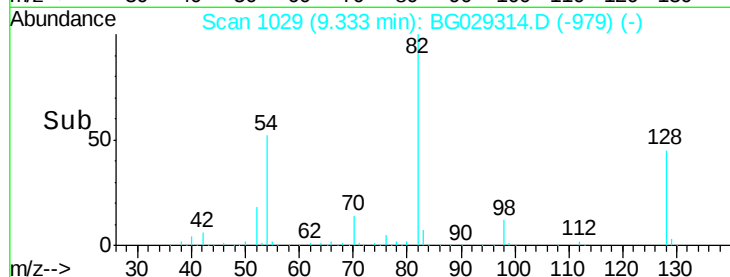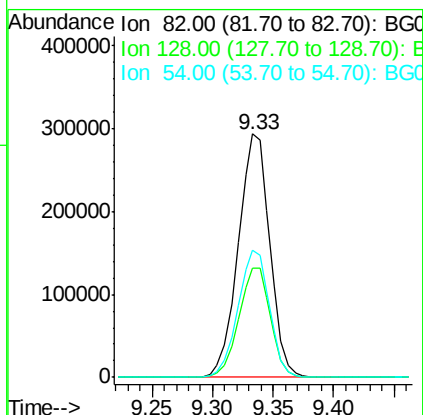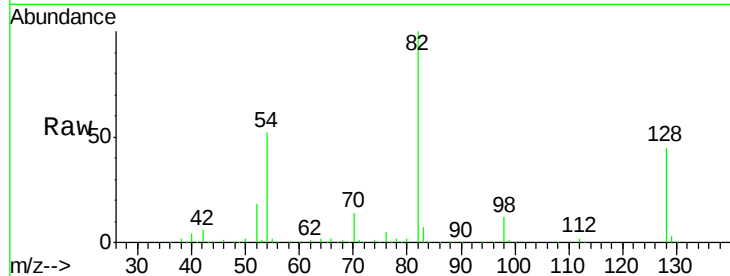

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.79 min Scan# 1957
 Delta R.T. -0.01 min
 Lab File: BG029314.D
 Acq: 17 Oct 2017 23:30

Tgt Ion: 164 Resp: 221670
 Ion Ratio Lower Upper
 164 100
 162 101.8 78.8 118.2
 160 44.5 35.4 53.0


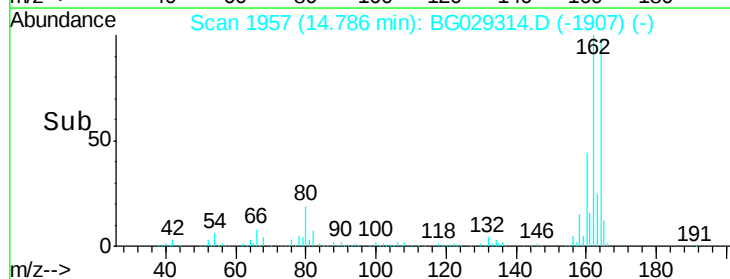
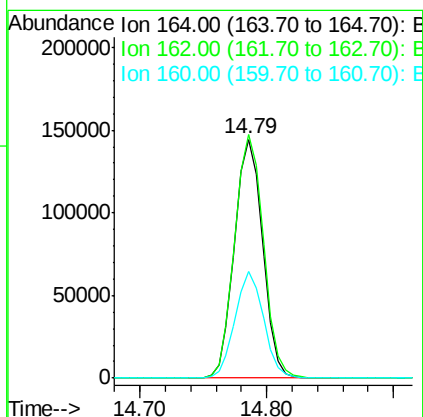
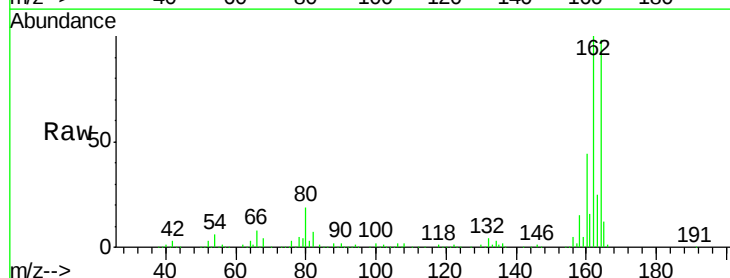


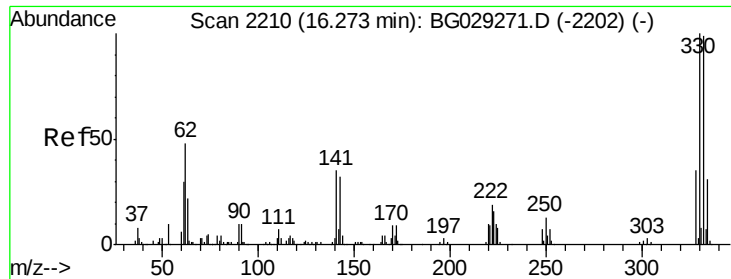

#41
 2,4,6-Tribromophenol
 Concen: 91.42 ng
 RT: 16.27 min Scan# 2209
 Delta R.T. -0.01 min
 Lab File: BG029314.D
 Acq: 17 Oct 2017 23:30




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion:330 Resp: 261640
 Ion Ratio Lower Upper
 330 100
 332 96.4 77.0 115.6
 141 33.9 25.2 37.8

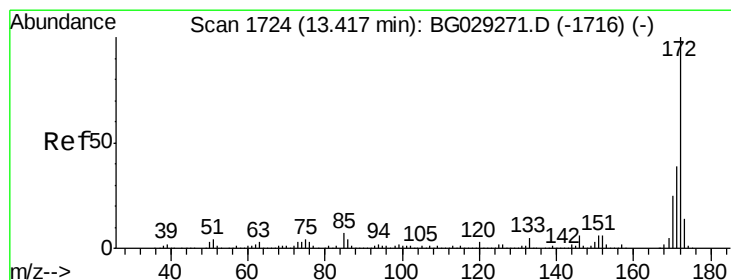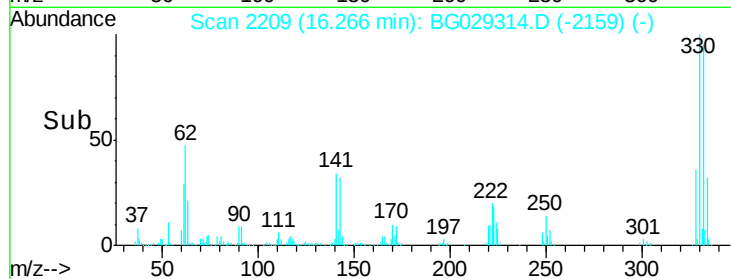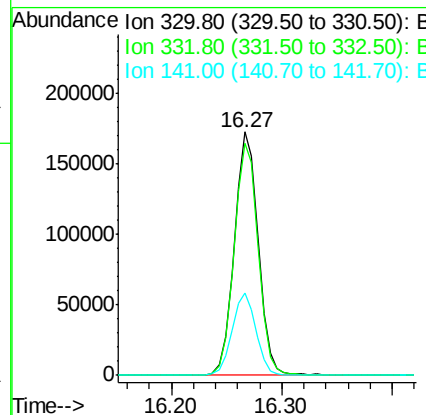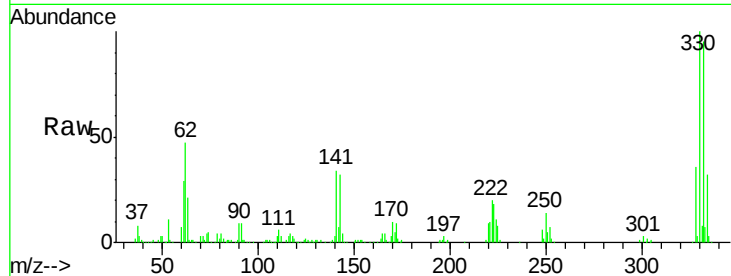

#44
 2-Fluorobiphenyl
 Concen: 91.82 ng
 RT: 13.42 min Scan# 1724
 Delta R.T. -0.00 min
 Lab File: BG029314.D
 Acq: 17 Oct 2017 23:30

Tgt Ion:172 Resp: 1387816
 Ion Ratio Lower Upper
 172 100
 171 39.2 30.0 45.0
 170 26.1 19.5 29.3

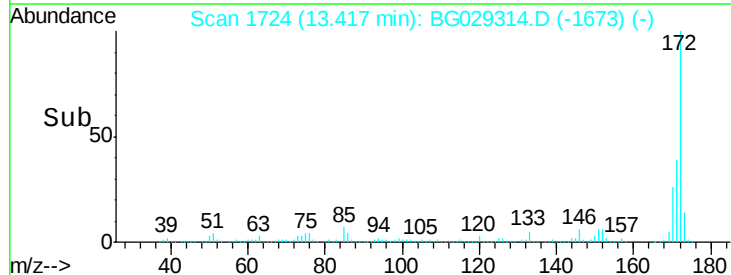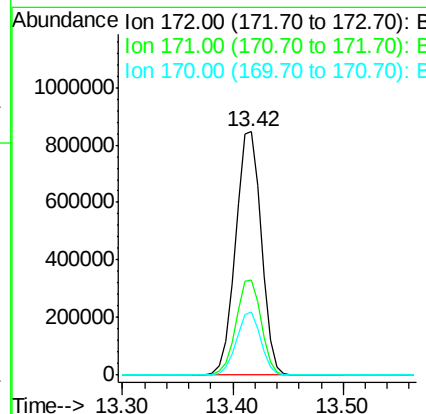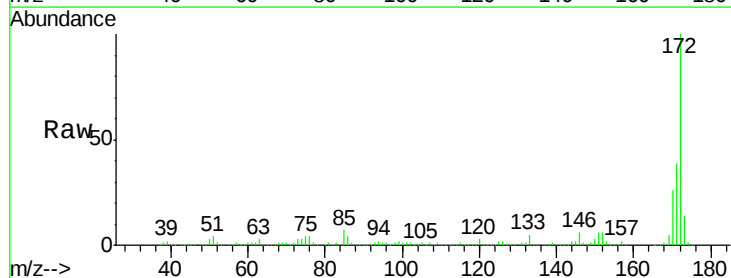


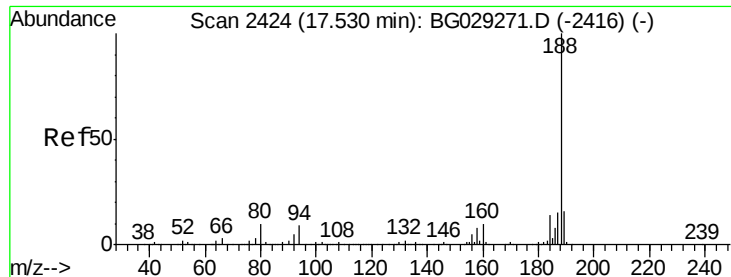




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.52 min Scan# 2423
Delta R.T. -0.01 min
Lab File: BG029314.D
Acq: 17 Oct 2017 23:30

Instrument :
BNA_G
ClientSampleId :

Tot Ion:188 Resp: 500068
Ion Ratio Lower Upper
188 100
94 8.5 6.9 10.3
80 9.8 7.7 11.5

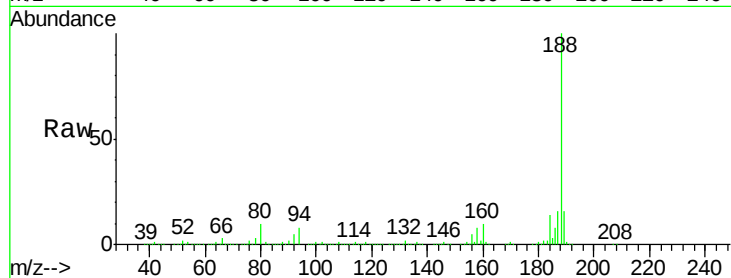


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

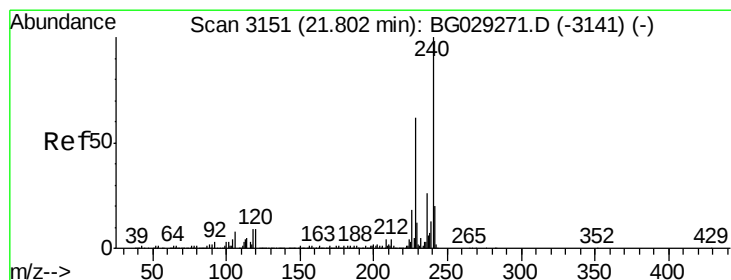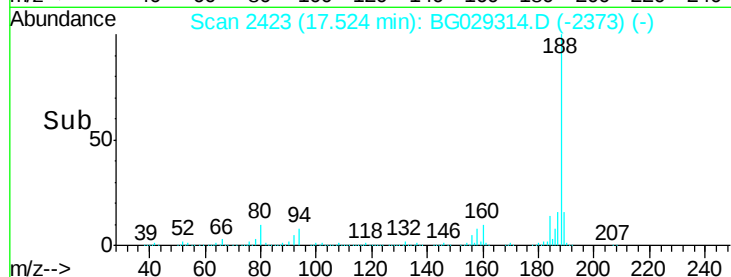
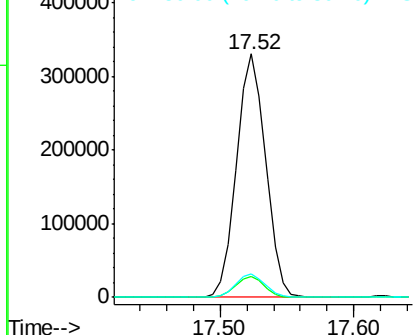



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.80 min Scan# 3150
Delta R.T. -0.01 min
Lab File: BG029314.D
Acq: 17 Oct 2017 23:30

Tgt Ion:240 Resp: 516800
Ion Ratio Lower Upper
240 100
120 9.6 6.8 10.2
236 26.7 20.9 31.3

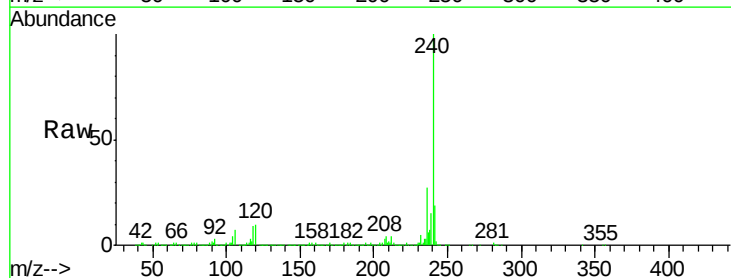

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



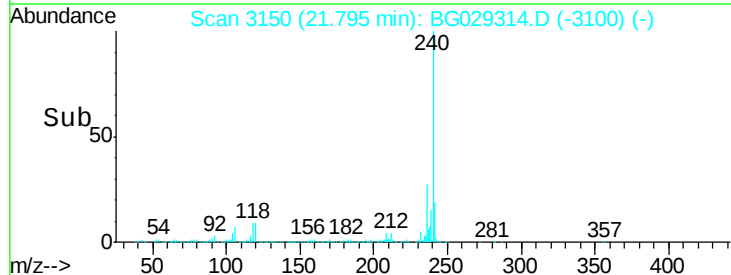
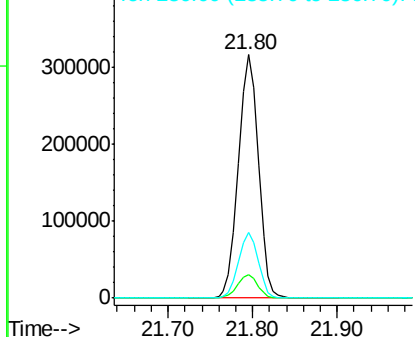


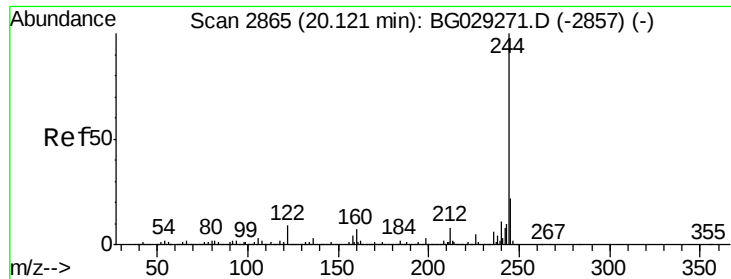

#78
 Terphenyl-d14
 Concen: 85.16 ng
 RT: 20.11 min Scan# 2864
 Delta R.T. -0.01 min
 Lab File: BG029314.D
 Acq: 17 Oct 2017 23:30

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:244 Resp: 1934641
 Ion Ratio Lower Upper
 244 100
 212 8.6 5.8 8.8
 122 10.4 7.0 10.4

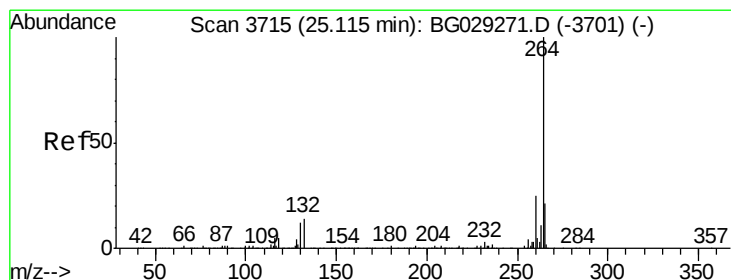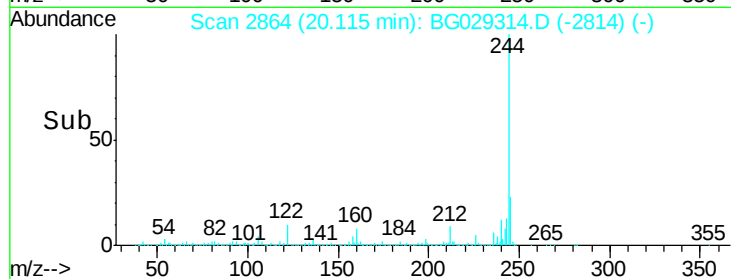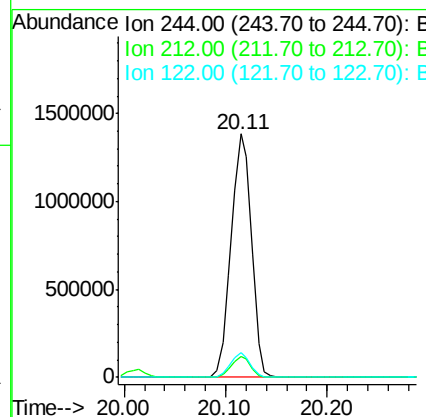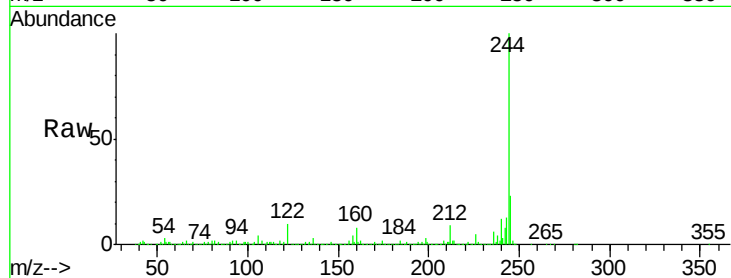

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 25.10 min Scan# 3713
 Delta R.T. -0.01 min
 Lab File: BG029314.D
 Acq: 17 Oct 2017 23:30

Tgt Ion:264 Resp: 537897
 Ion Ratio Lower Upper
 264 100
 260 24.1 17.4 26.0
 265 22.1 17.7 26.5

