


Data Path : Z:\HPCHEM1\BNA G\Data\BG101717\
 Data File : BG029300.D
 Acq On : 17 Oct 2017 14:14
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG101617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 16 17:32:15 2017

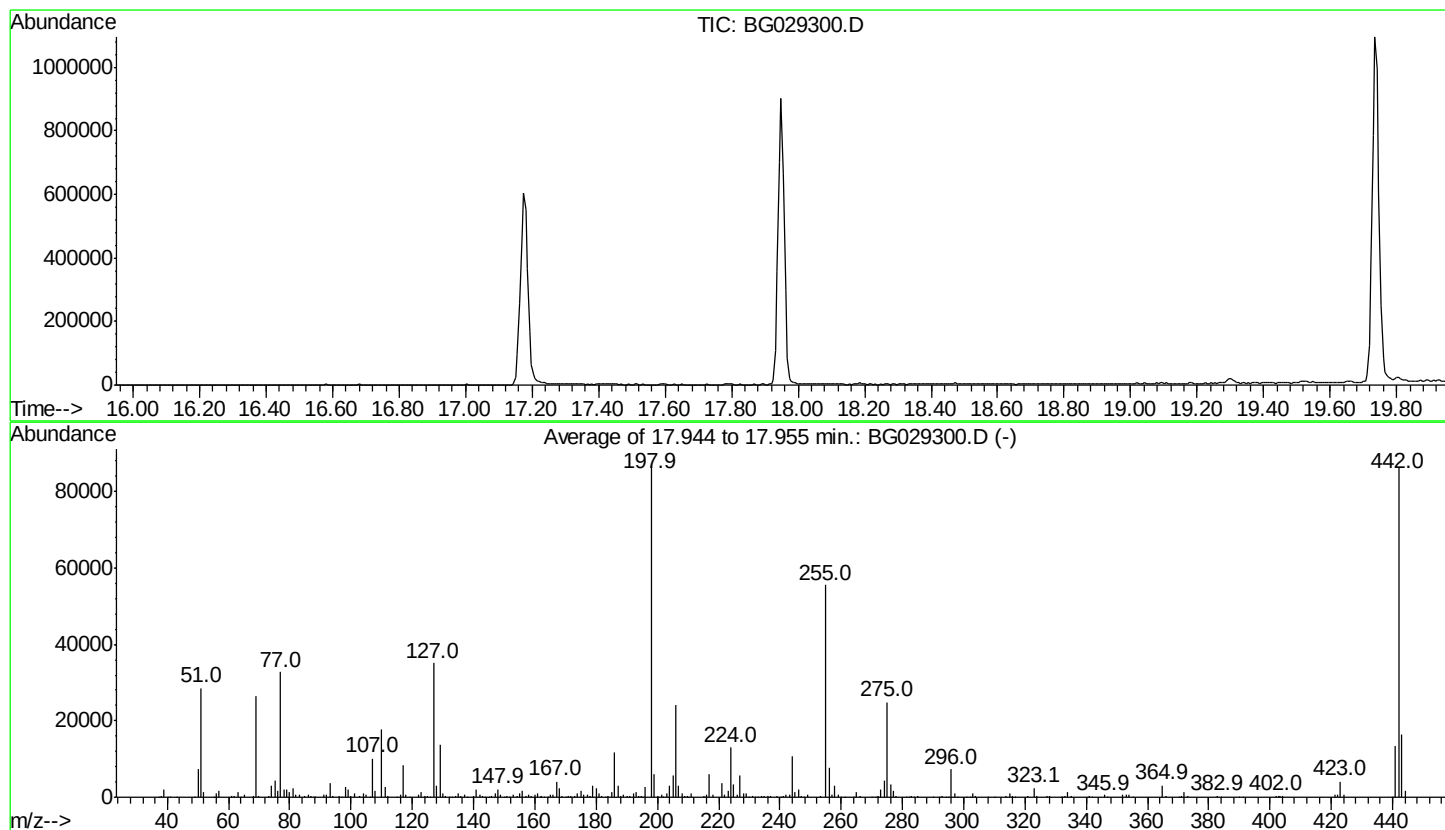

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	28490	PASS
68	69	0.00	2	0.9	252	PASS
69	198	0.00	100	30.7	26600	PASS
70	69	0.00	2	0.8	212	PASS
127	198	10	80	40.4	35085	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	86781	PASS
199	198	5	9	7.0	6101	PASS
275	198	10	60	28.7	24885	PASS
365	198	1	100	3.6	3165	PASS
441	442	0.01	24	15.6	13525	PASS
442	198	50	100	99.6	86474	PASS
443	442	15	24	19.2	16589	PASS