


Data Path : Z:\HPCHEM1\BNA G\Data\BG101717\
 Data File : BG029319.D
 Acq On : 18 Oct 2017 2:48
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG101617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 16 17:32:15 2017

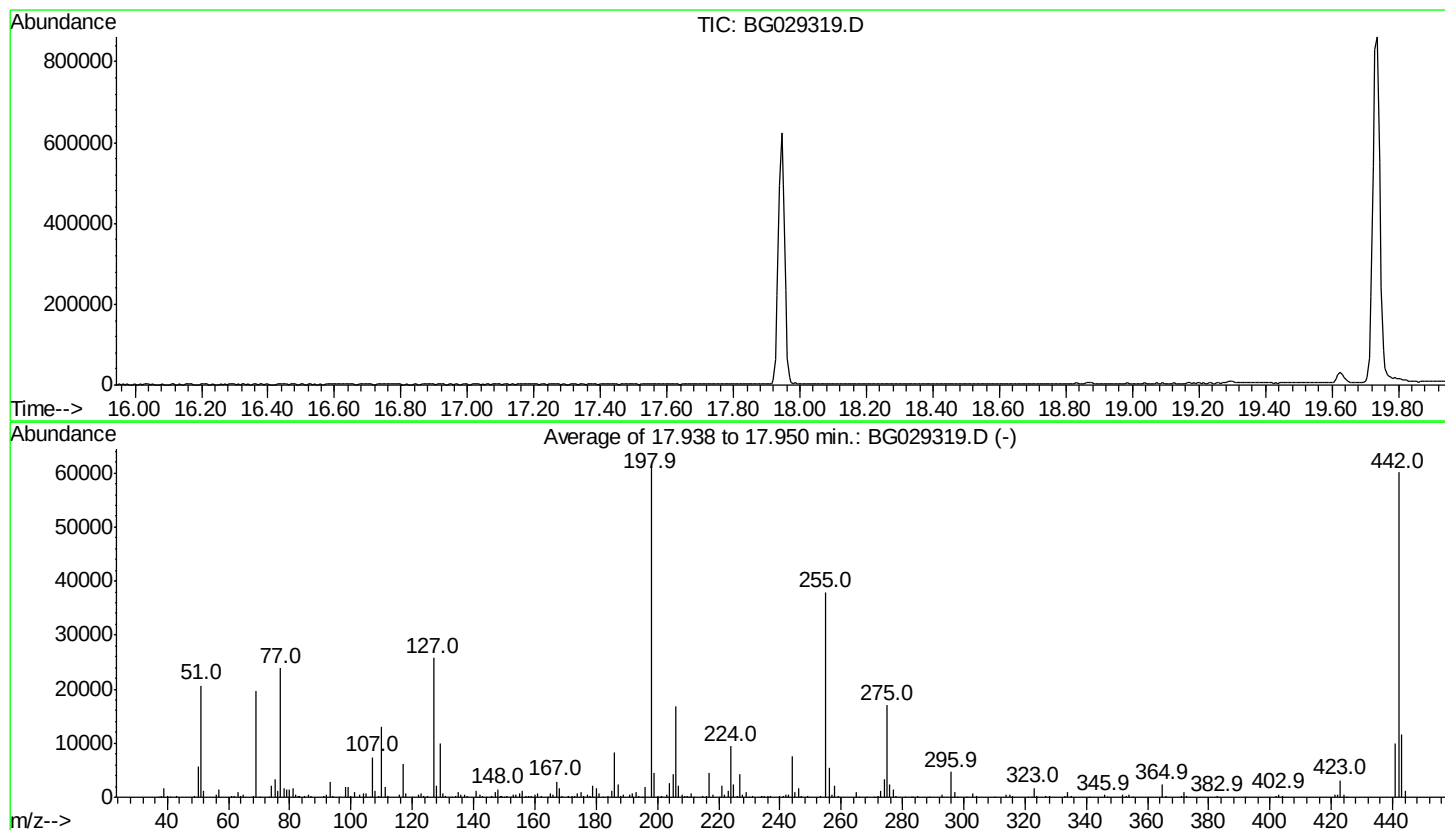

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	20653	PASS
68	69	0.00	2	1.1	208	PASS
69	198	0.00	100	32.2	19752	PASS
70	69	0.00	2	0.3	51	PASS
127	198	10	80	42.0	25768	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61333	PASS
199	198	5	9	7.3	4454	PASS
275	198	10	60	27.7	17017	PASS
365	198	1	100	3.8	2307	PASS
441	442	0.01	24	16.6	9954	PASS
442	198	50	100	97.9	60064	PASS
443	442	15	24	19.3	11599	PASS