


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101718\
 Data File : BG037391.D
 Acq On : 17 Oct 2018 15:34
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 17 15:19:35 2018

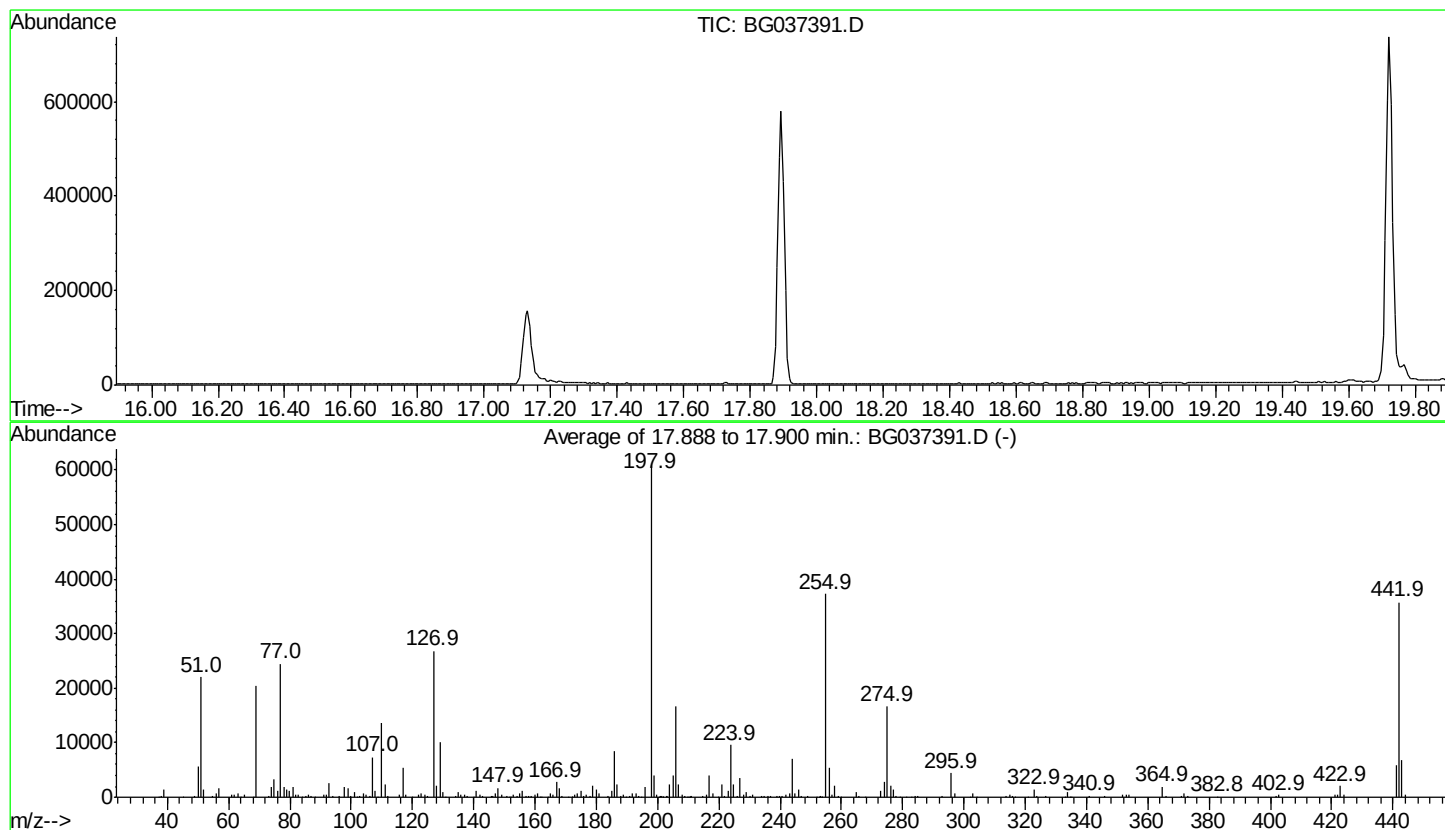

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	21996	PASS
68	69	0.00	2	0.5	101	PASS
69	198	0.00	100	33.6	20403	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.1	26797	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60810	PASS
199	198	5	9	6.7	4051	PASS
275	198	10	60	27.4	16654	PASS
365	198	1	100	3.3	1995	PASS
441	198	0.01	100	9.6	5827	PASS
442	198	50	100	58.7	35722	PASS
443	442	15	24	18.9	6751	PASS