

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101720\
 Data File : BG046944.D
 Acq On : 17 Oct 2020 16:17
 Operator : CG/JU
 Sample : L4259-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C5CG2

Manual Integrations
 APPROVED

mohammad
 10/19/2020 1:25:50 PM

Quant Time: Oct 19 01:28:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG101520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 19 00:57:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	64439	20.00	ng/ul	0.00
18) Naphthalene-d8	10.88	136	265589	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.70	164	186059	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.45	188	397447	20.00	ng/ul	0.00
78) Chrysene-d12	21.72	240	384987	20.00	ng/ul	0.00
86) Perylene-d12	24.96	264	387843	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.48	96	1481	1.02	ng/uL	0.00
5) Phenol-d5	7.22	99	40509	7.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.39	67	96713	29.37	ng/ul	0.00
9) 2-Chlorophenol-d4	7.60	132	108031	25.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.77	113	76383	16.83	ng/ul	0.00
19) Nitrobenzene-d5	9.23	128	70311m	31.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.96	143	82017	31.86	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.50	165	153831	30.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.99	131	9613	1.66	ng/ul	-0.02
44) Dimethylphthalate-d6	14.10	166	526992	34.10	ng/ul	0.00
47) Acenaphthylene-d8	14.40	160	607068	34.46	ng/ul	0.00
52) 4-Nitrophenol-d4	14.89	143	19760	7.42	ng/ul	0.00
58) Fluorene-d10	15.69	176	471547	33.19	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.81	200	133261	48.69	ng/ul	0.00
71) Anthracene-d10	17.55	188	707087	36.73	ng/ul	0.00
79) Pyrene-d10	19.83	212	820742	38.89	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.74	264	794255	36.36	ng/ul	0.00

Target Compounds

					Ovalue	
14) Acetophenone	8.88	105	18616	2.557	ng/ul#	44
40) 2,4,5-Trichlorophenol	13.21	196	16204	3.437	ng/ul	90
45) Dimethylphthalate	14.15	163	21952	1.370	ng/ul#	90
50) Acenaphthene	14.77	153	16500	1.321	ng/ul	93
56) 2,3,4,6-Tetrachlorophenol	15.32	232	225623	48.318	ng/ul#	93
69) Pentachlorophenol	17.13	266	3924517	1145.051	ng/ul	89
80) Pyrene	19.85	202	60165	2.309	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101720\
Data File : BG046944.D
Acq On : 17 Oct 2020 16:17
Operator : CG/JU
Sample : L4259-14
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
C5CG2

Quant Time: Oct 19 01:28:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG101520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 19 00:57:03 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
10/19/2020 1:25:50 PM

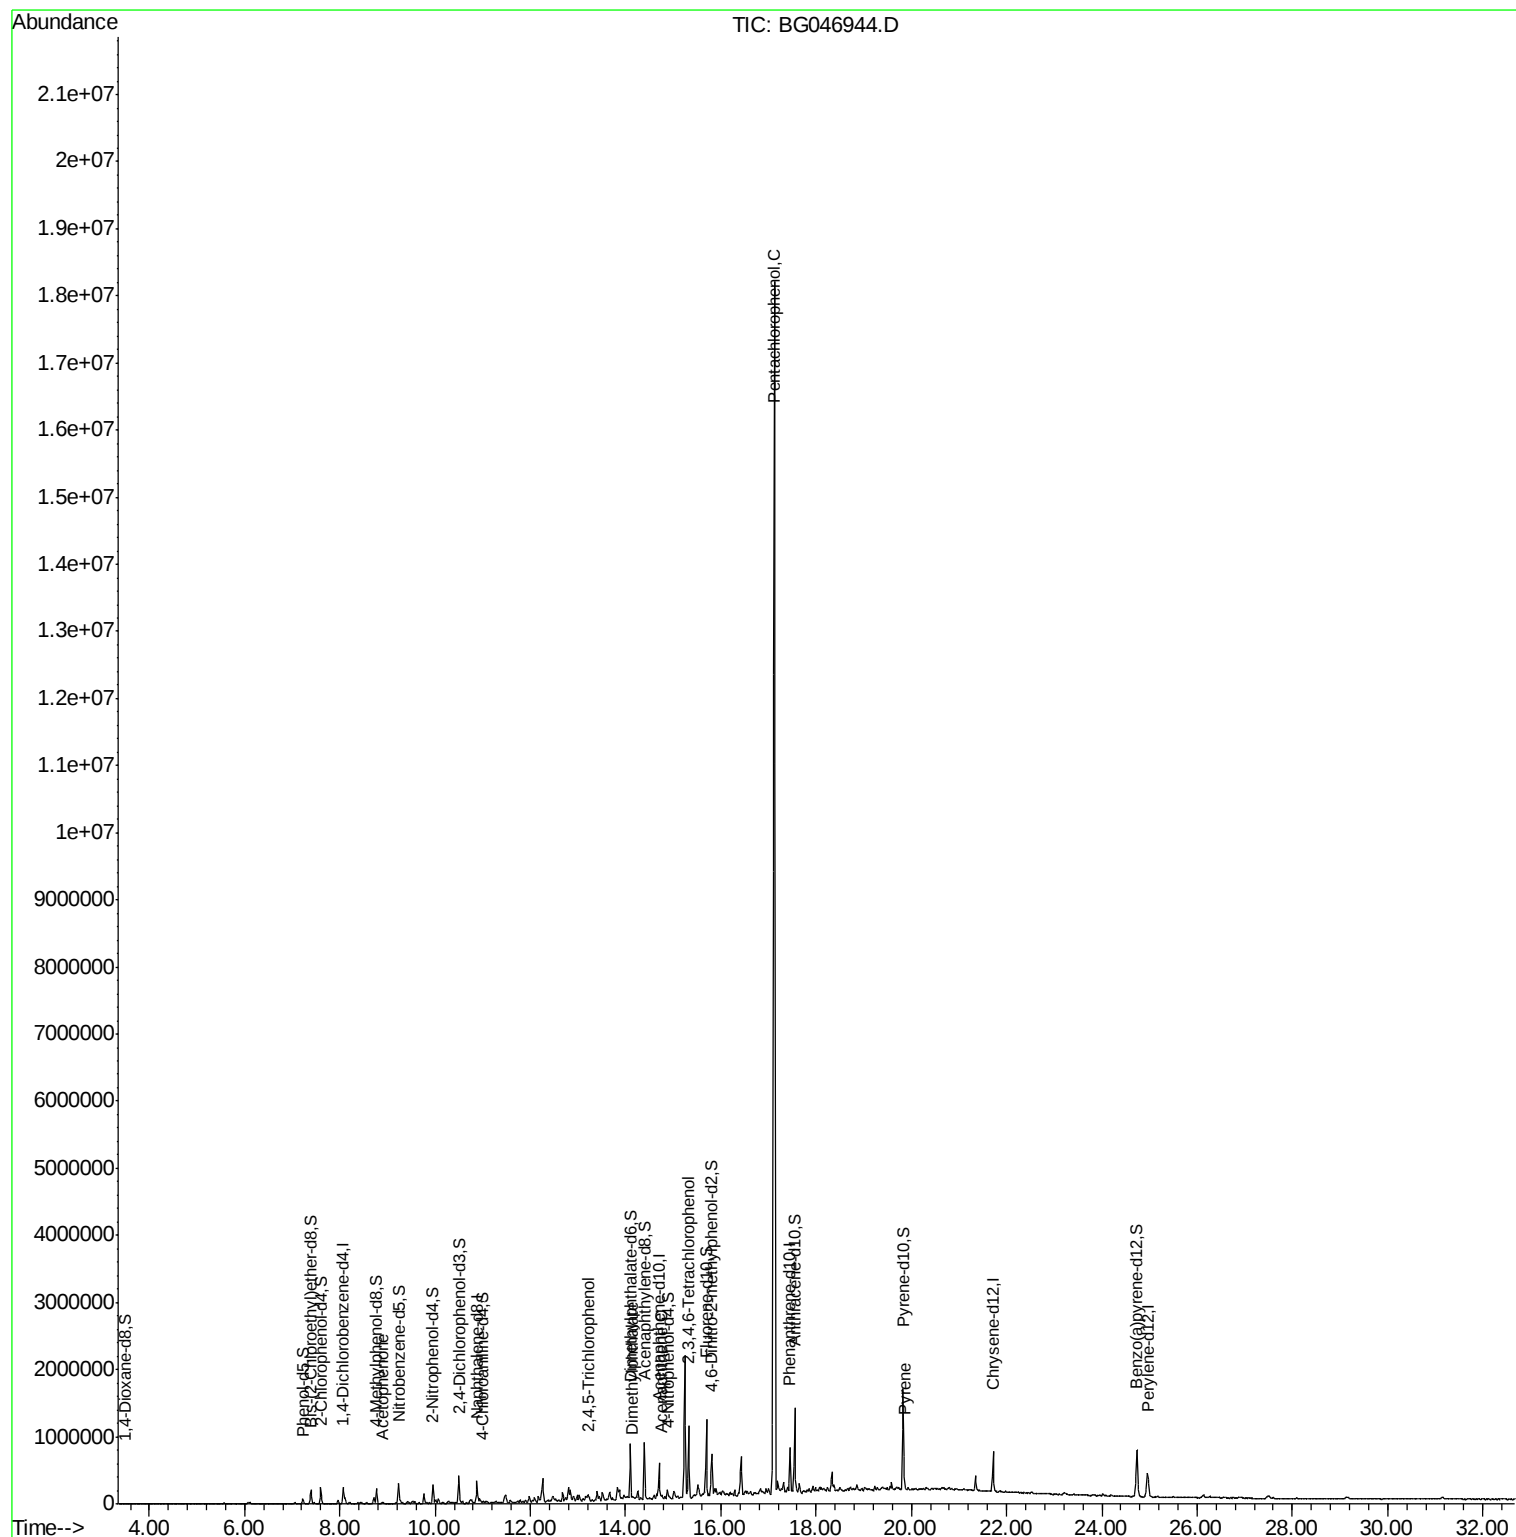

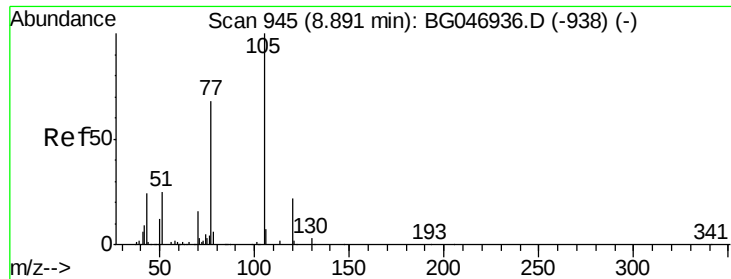





#14
Acetophenone
Concen: 2.557 ng/ul
RT: 8.88 min Scan# 943
Delta R.T. -0.01 min
Lab File: BG046944.D
Acq: 17 Oct 2020 16:17

Instrument :
BNA_G
ClientSampleId :
C5CG2

Tot Ion	Ratio	Resp Lower	Upper
105	100		
77	24.6	64.7	97.1#
51	11.5	26.5	39.7#




Manual Integrations
APPROVED


mohammad
10/19/2020 1:25:50 PM

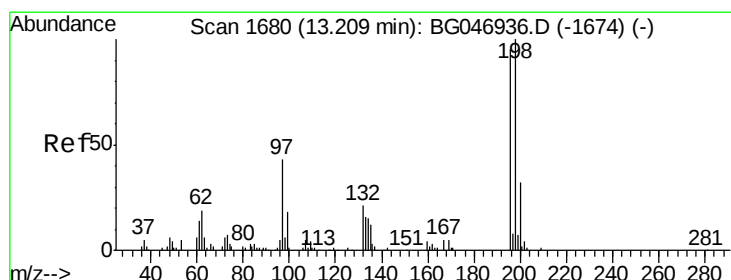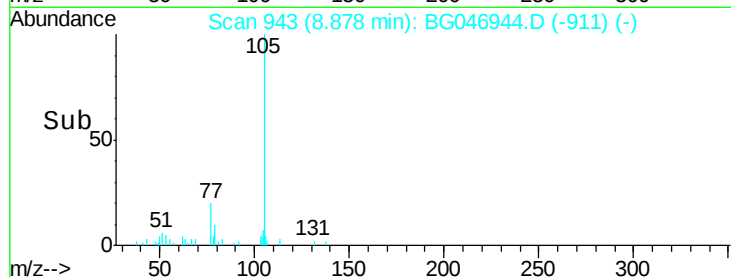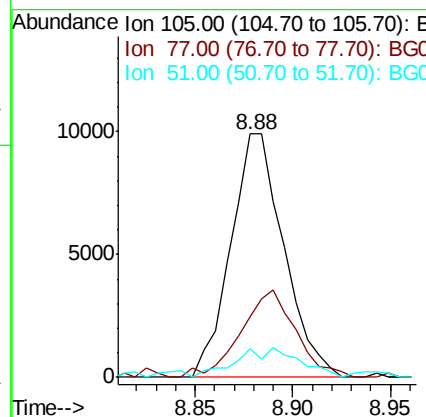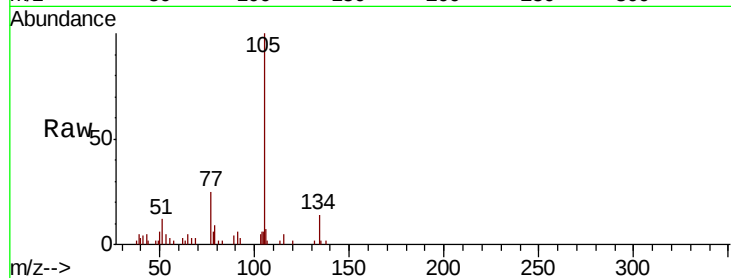

#40
2,4,5-Trichlorophenol
Concen: 3.437 ng/ul
RT: 13.21 min Scan# 1680
Delta R.T. -0.00 min
Lab File: BG046944.D
Acq: 17 Oct 2020 16:17

Tgt Ion	Ratio	Resp Lower	Upper
196	100		
198	91.4	82.4	123.6
200	30.7	26.3	39.5

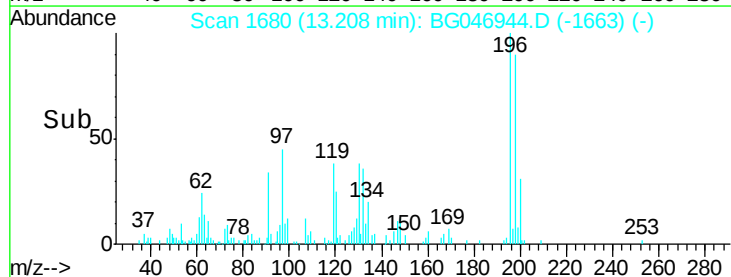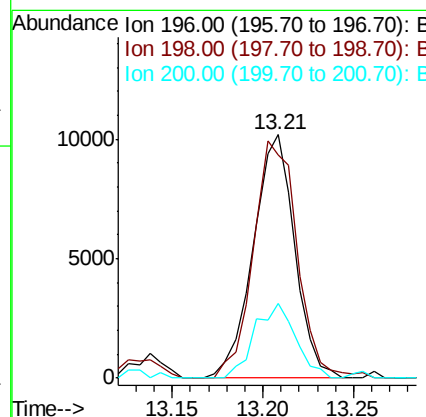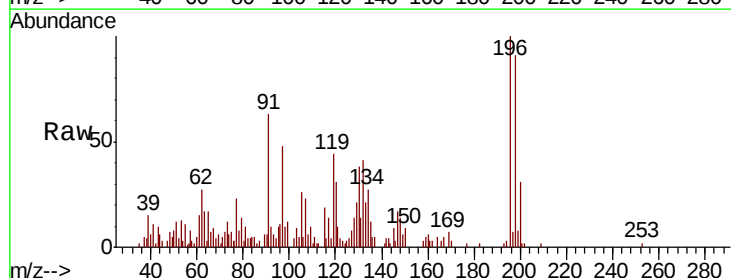

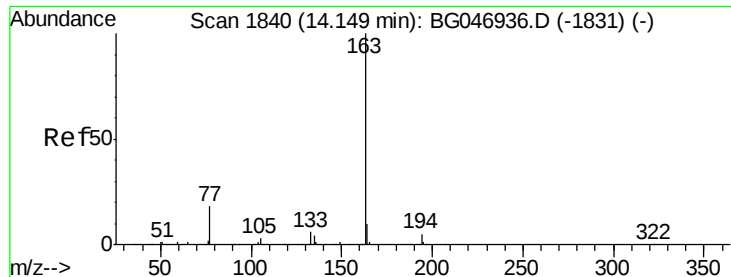


#45
Dimethylphthalate
Concen: 1.370 ng/ul
RT: 14.15 min Scan# 1840
Delta R.T. -0.00 min
Lab File: BG046944.D
Acq: 17 Oct 2020 16:17

Instrument :
BNA_G
ClientSampleId :
C5CG2

Tot Ion	Ratio	Resp	Lower	Upper
163	100	21952		
194	5.4		3.9	5.9
164	14.8		7.8	11.8

Manual Integrations
APPROVED

mohammad
10/19/2020 1:25:50 PM



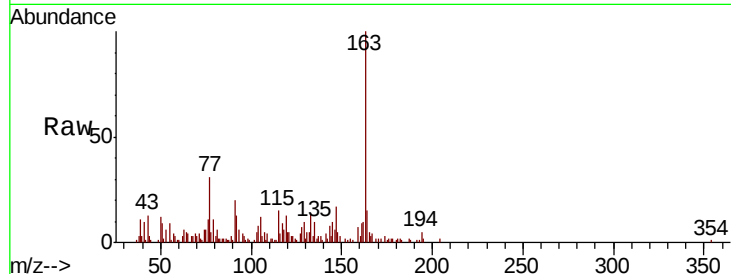


Abundance

Ion 163.00 (162.70 to 163.70): E


Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

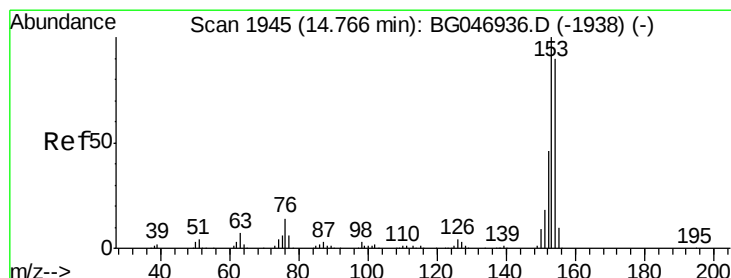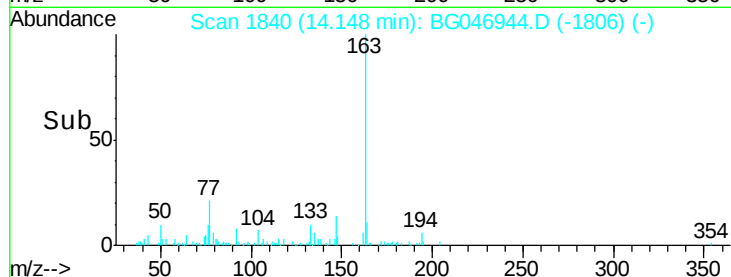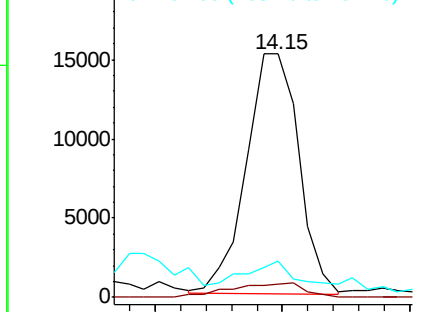

#50
Acenaphthene
Concen: 1.321 ng/ul
RT: 14.77 min Scan# 1945
Delta R.T. -0.00 min
Lab File: BG046944.D
Acq: 17 Oct 2020 16:17

Tgt Ion	Ratio	Resp	Lower	Upper
153	100	16500		
152	52.4		39.0	58.6
154	82.1		71.6	107.4


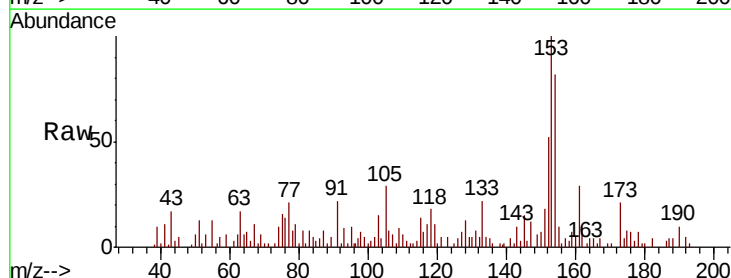



Abundance

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

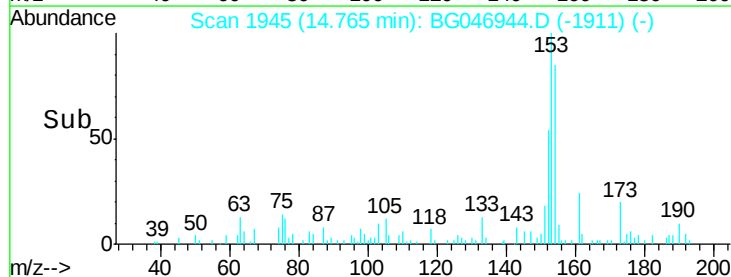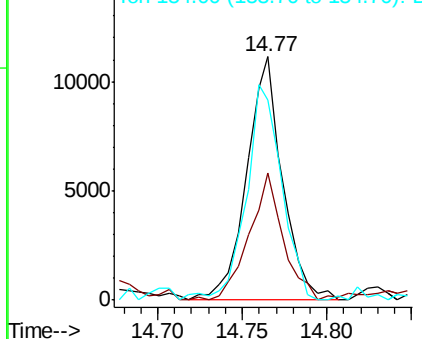

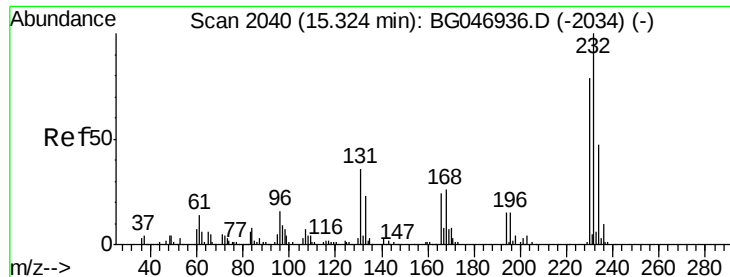





#56
 2,3,4,6-Tetrachlorophenol
 Concen: 48.318 ng/ul
 RT: 15.32 min Scan# 2040
 Delta R.T. -0.00 min
 Lab File: BG046944.D
 Acq: 17 Oct 2020 16:17

Instrument :
 BNA_G
 ClientSampleId :
 C5CG2

Tot Ion	Ion	Ratio	Resp	Lower	Upper
232	100		225623		
131	38.3	26.2	39.4		
130	3.1	0.0	0.0		
166	26.3	22.5	33.7		




Manual Integrations
 APPROVED


mohammad
 10/19/2020 1:25:50 PM

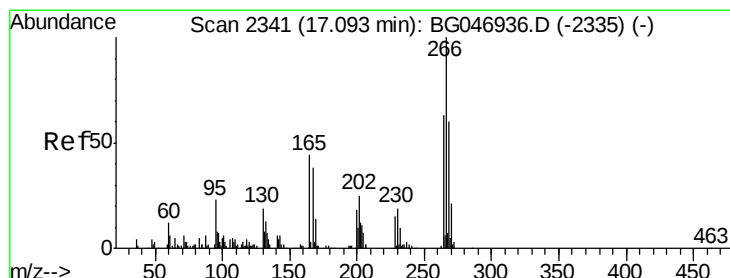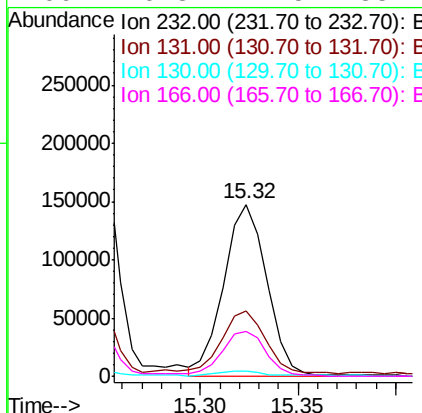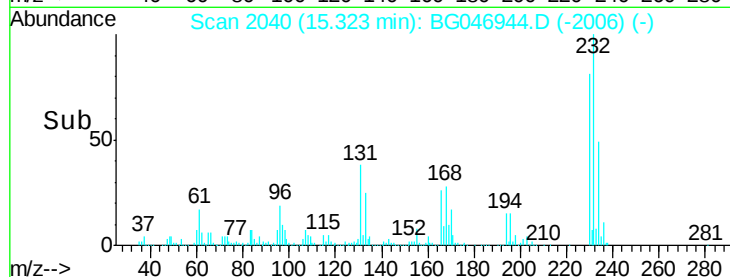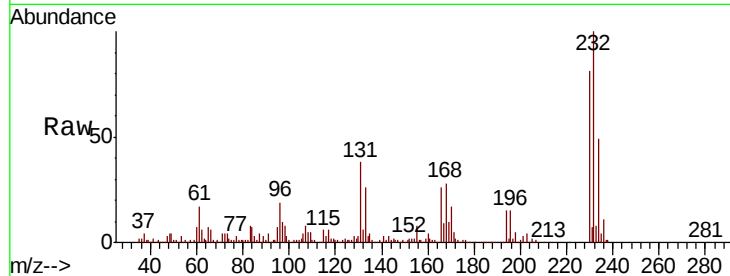

#69
 Pentachlorophenol
 Concen: 1145.051 ng/ul
 RT: 17.13 min Scan# 2347
 Delta R.T. 0.03 min
 Lab File: BG046944.D
 Acq: 17 Oct 2020 16:17

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
266	100		3924517		
264	74.4	52.6	78.8		
268	74.3	52.2	78.2		

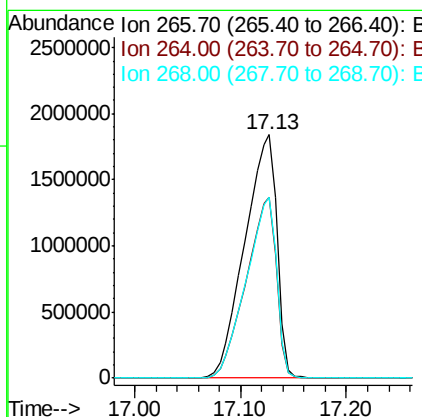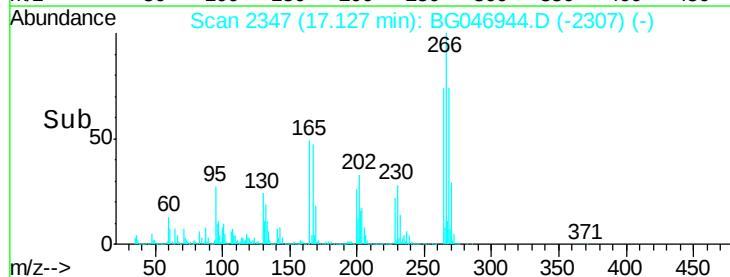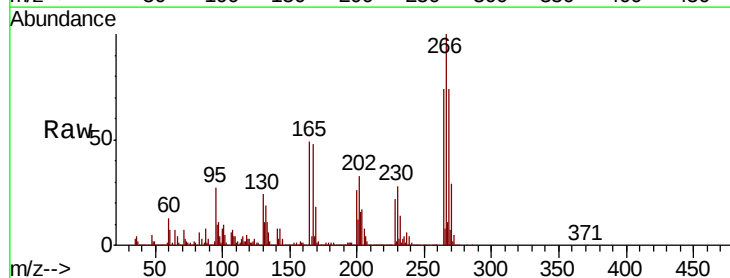

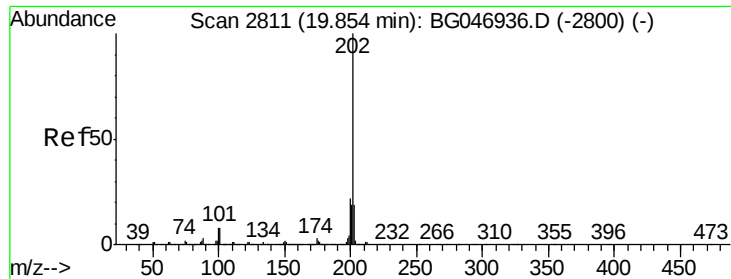

#80
 Pvrene
 Concen: 2.309 ng/ul
 RT: 19.85 min Scan# 2811
 Delta R.T. -0.00 min
 Lab File: BG046944.D
 Acq: 17 Oct 2020 16:17

Instrument :
 BNA_G
 ClientSampleId :
 C5CG2

Tot Ion:	202	Resp:	60165
Ion Ratio	Lower	Upper	
202	100		
101	7.7	6.5	9.7
100	7.6	5.2	7.8

Manual Integrations
 APPROVED

mohammad
 10/19/2020 1:25:50 PM

