

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101722\
 Data File : BG055191.D
 Acq On : 17 Oct 2022 12:10
 Operator : CG/JU
 Sample : PB148341BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB148341BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG055191.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.821	423	431	440	rBV	313354	508651	21.99%	6.487%
2	7.437	697	706	716	rBV	325611	563672	24.37%	7.188%
3	8.300	847	853	860	rVB	67033	109417	4.73%	1.395%
4	9.470	1045	1052	1062	rBV	191489	342221	14.80%	4.364%
5	11.132	1327	1335	1343	rBV	96400	171563	7.42%	2.188%
6	13.541	1738	1745	1758	rVB	623766	943670	40.80%	12.034%
7	14.910	1971	1978	1985	rBV	186037	287728	12.44%	3.669%
8	16.385	2223	2229	2246	rBV	542743	884364	38.24%	11.278%
9	17.648	2437	2444	2454	rBV	301952	464252	20.07%	5.920%
10	19.899	2822	2827	2832	rBV2	23193	25691	1.11%	0.328%
11	20.222	2876	2882	2888	rBV	1803418	2312785	100.00%	29.494%
12	21.931	3166	3173	3180	rBV	320544	557946	24.12%	7.115%
13	25.357	3746	3756	3769	rVB	226062	669644	28.95%	8.540%




Sum of corrected areas: 7841604

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101722\
Data File : BG055191.D
Acq On : 17 Oct 2022 12:10
Operator : CG/JU
Sample : PB148341BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB148341BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

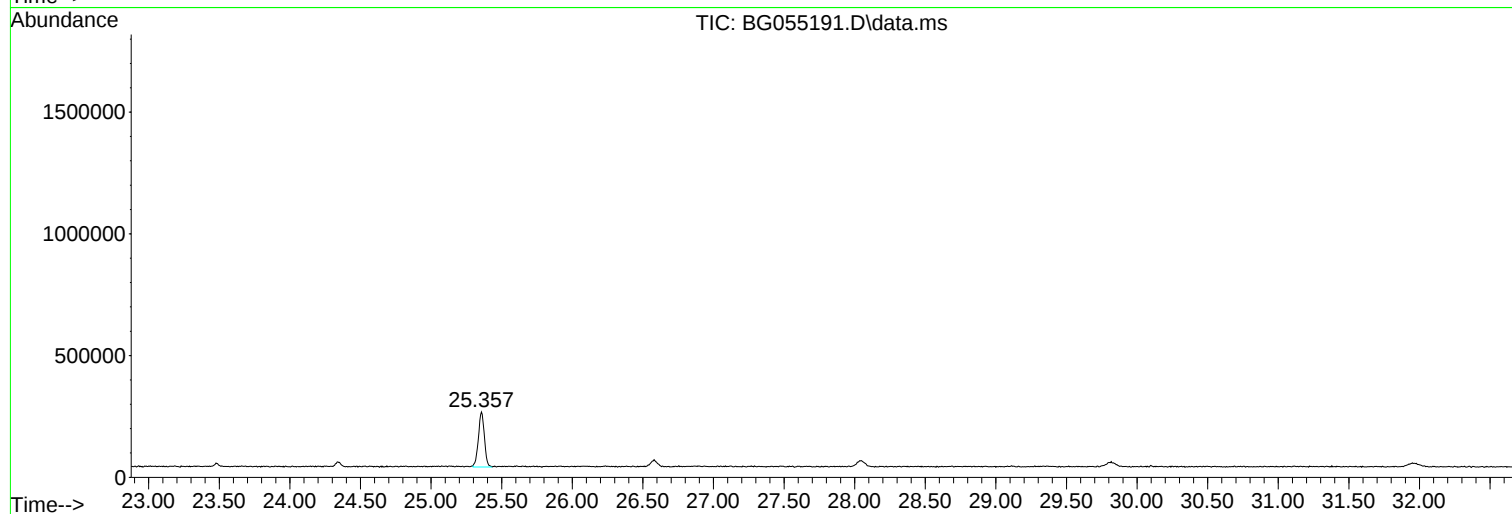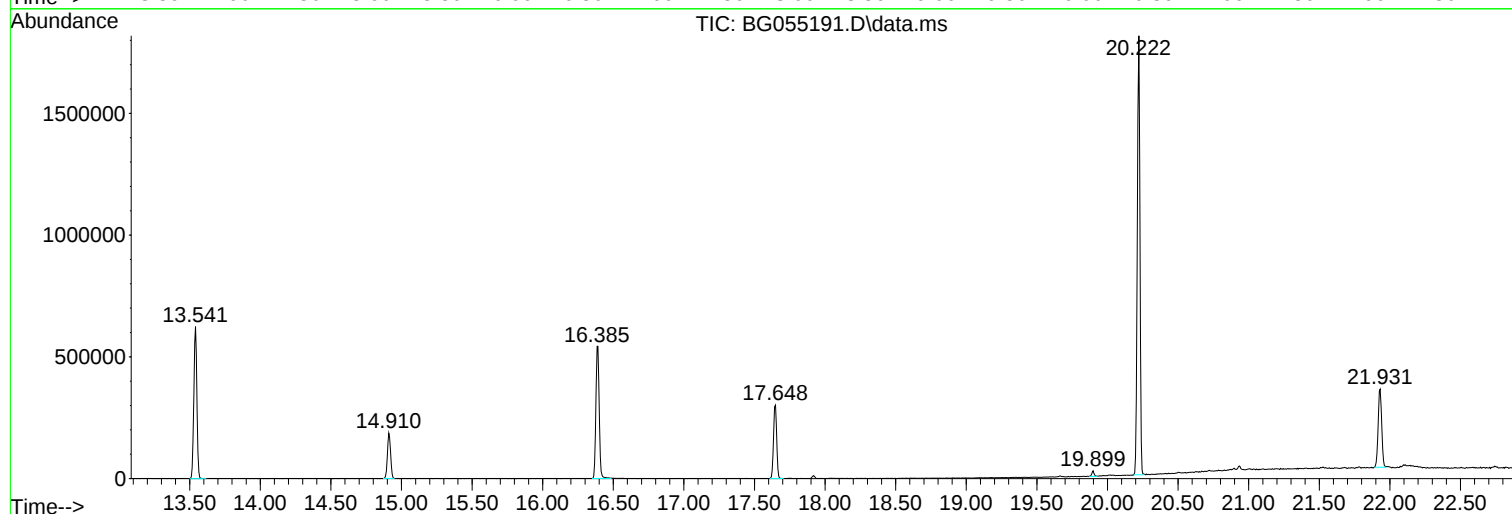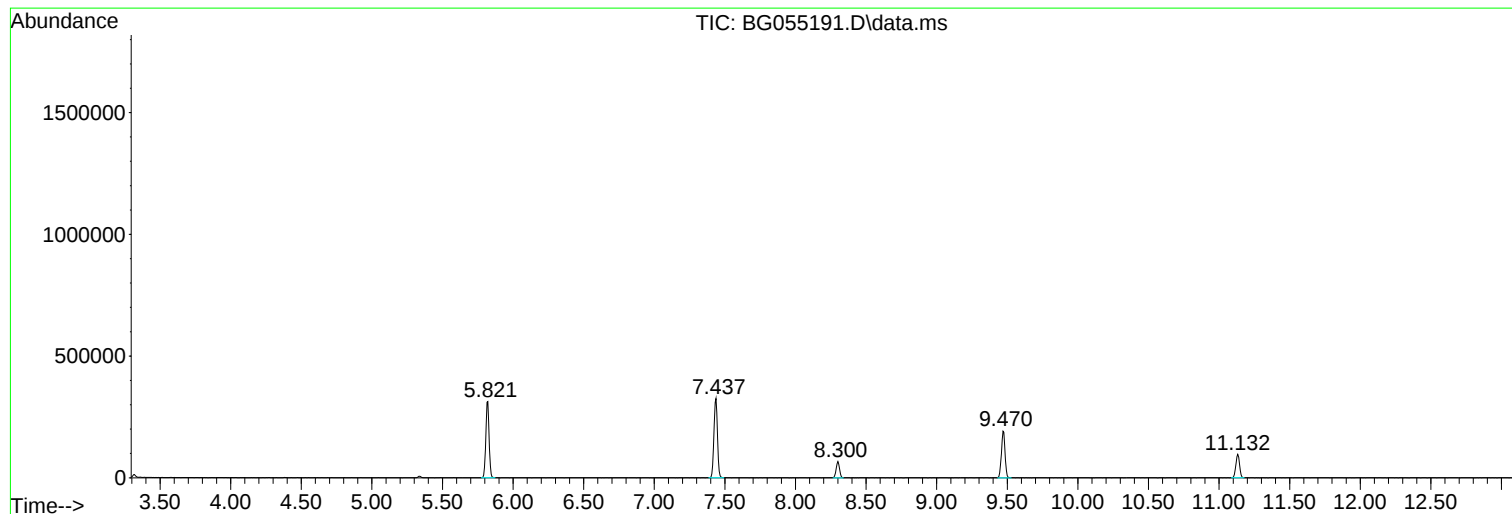

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101722\
Data File : BG055191.D
Acq On : 17 Oct 2022 12:10
Operator : CG/JU
Sample : PB148341BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB148341BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101722\
Data File : BG055191.D
Acq On : 17 Oct 2022 12:10
Operator : CG/JU
Sample : PB148341BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB148341BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------