

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101722\
 Data File : BG055199.D
 Acq On : 17 Oct 2022 19:28
 Operator : CG/JU
 Sample : N5150-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 WC-C2(0-6)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG055199.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.318	3	5	11	rVB	224213	287521	13.06%	2.569%
2	5.339	343	349	358	rVB	92562	147461	6.70%	1.318%
3	5.821	424	431	442	rVB	494971	795966	36.16%	7.112%
4	7.437	697	706	720	rBV	507938	891443	40.50%	7.965%
5	8.300	846	853	866	rVB	94366	159484	7.25%	1.425%
6	9.469	1045	1052	1061	rBV	313133	550306	25.00%	4.917%
7	10.874	1283	1291	1298	rBV	20763	34220	1.55%	0.306%
8	11.126	1326	1334	1344	rBV	129731	237546	10.79%	2.122%
9	13.541	1737	1745	1752	rBV	904349	1427607	64.85%	12.756%
10	14.910	1971	1978	1985	rVB	237168	368279	16.73%	3.291%
11	16.385	2222	2229	2242	rBV	813438	1254643	57.00%	11.210%
12	17.642	2437	2443	2447	rBV	317891	477770	21.70%	4.269%
13	17.683	2447	2450	2456	rVB	86407	119330	5.42%	1.066%
14	17.748	2456	2461	2464	rBV2	17024	24527	1.11%	0.219%
15	18.506	2583	2590	2594	rBV3	19229	39622	1.80%	0.354%
16	18.559	2594	2599	2608	rVB2	17492	30026	1.36%	0.268%
17	18.706	2617	2624	2628	rBV3	16969	36892	1.68%	0.330%
18	19.669	2783	2788	2795	rVB	162353	233756	10.62%	2.089%
19	19.998	2839	2844	2845	rBV2	24538	31334	1.42%	0.280%
20	20.034	2845	2850	2856	rVB	139528	209918	9.54%	1.876%
21	20.216	2875	2881	2887	rBV	1705882	2201241	100.00%	19.668%
22	20.515	2929	2932	2937	rVB2	19704	27925	1.27%	0.250%
23	21.520	3099	3103	3109	rVB3	54517	86887	3.95%	0.776%
24	21.925	3164	3172	3177	rBV2	301995	608105	27.63%	5.433%
25	21.972	3177	3180	3189	rVB	59813	99388	4.52%	0.888%
26	23.136	3374	3378	3386	rVB3	25862	50192	2.28%	0.448%
27	24.258	3561	3569	3577	rBV2	40708	145839	6.63%	1.303%
28	25.186	3720	3727	3738	rVB2	36287	101673	4.62%	0.908%
29	25.351	3745	3755	3765	rBV	176578	512995	23.30%	4.584%




Sum of corrected areas: 11191896

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101722\
Data File : BG055199.D
Acq On : 17 Oct 2022 19:28
Operator : CG/JU
Sample : N5150-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-C2(0-6)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

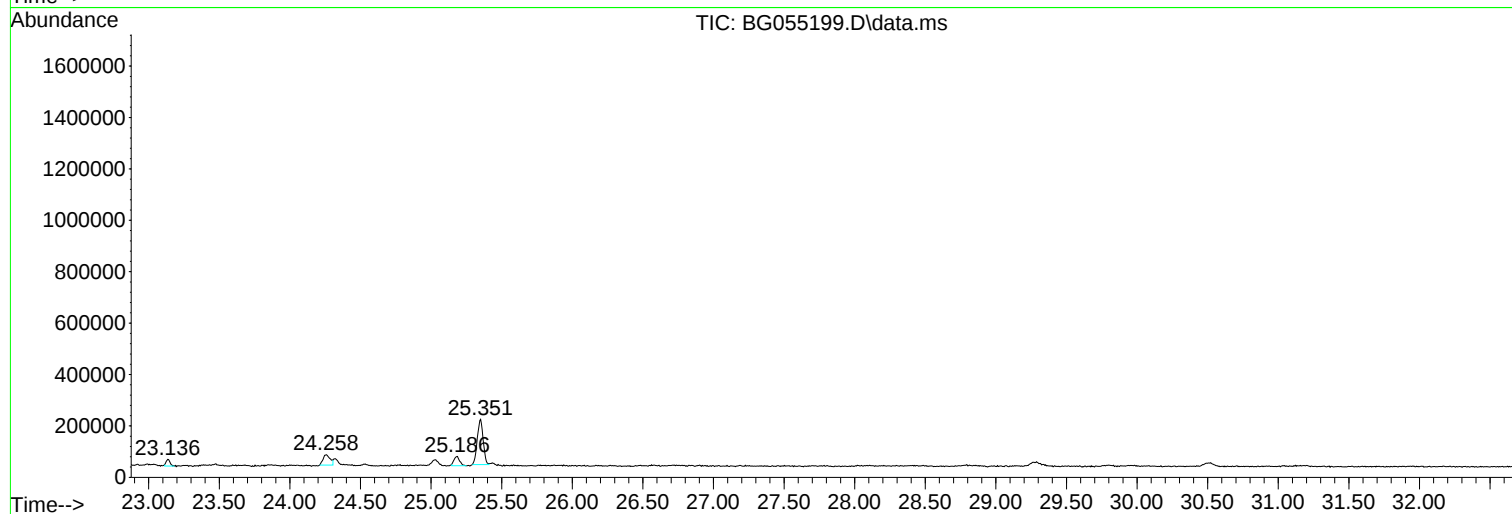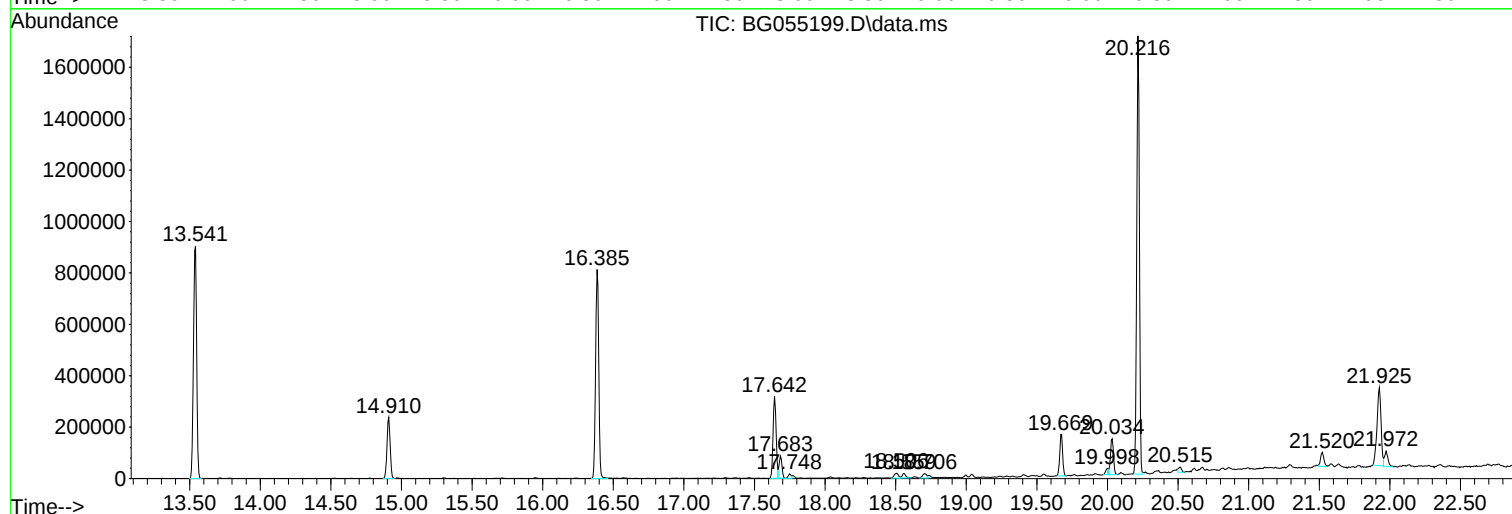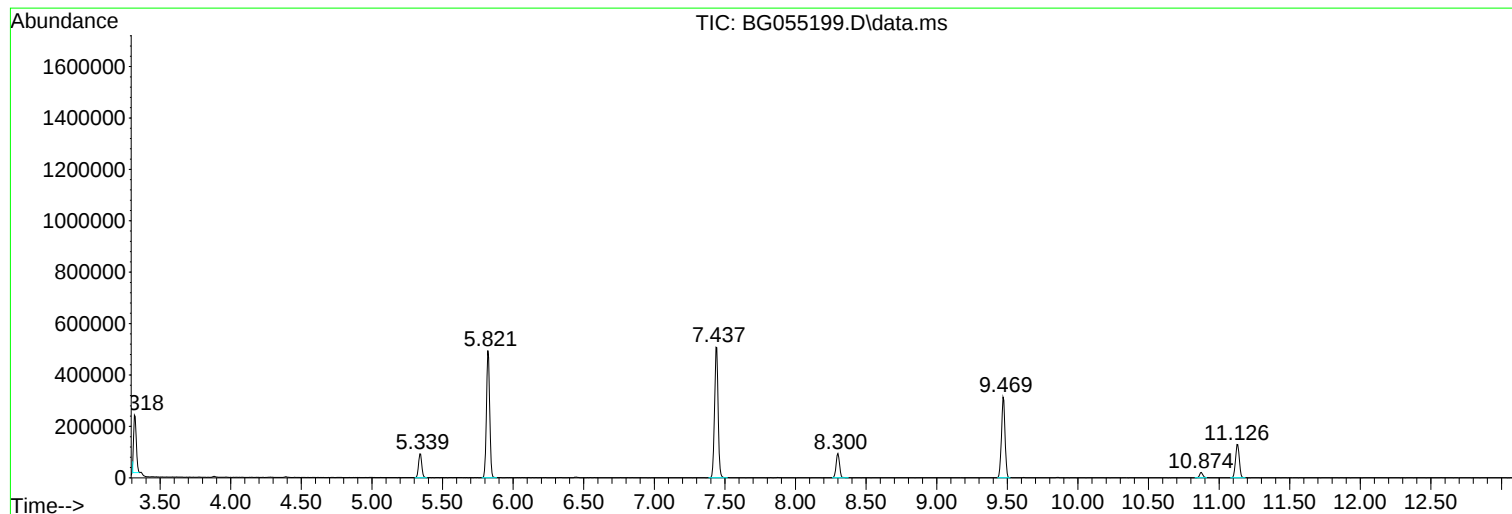

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101722\
Data File : BG055199.D
Acq On : 17 Oct 2022 19:28
Operator : CG/JU
Sample : N5150-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-C2(0-6)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101722\
Data File : BG055199.D
Acq On : 17 Oct 2022 19:28
Operator : CG/JU
Sample : N5150-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-C2(0-6)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------