


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101722\
 Data File : BG055189.D
 Acq On : 17 Oct 2022 10:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 13 05:14:13 2022

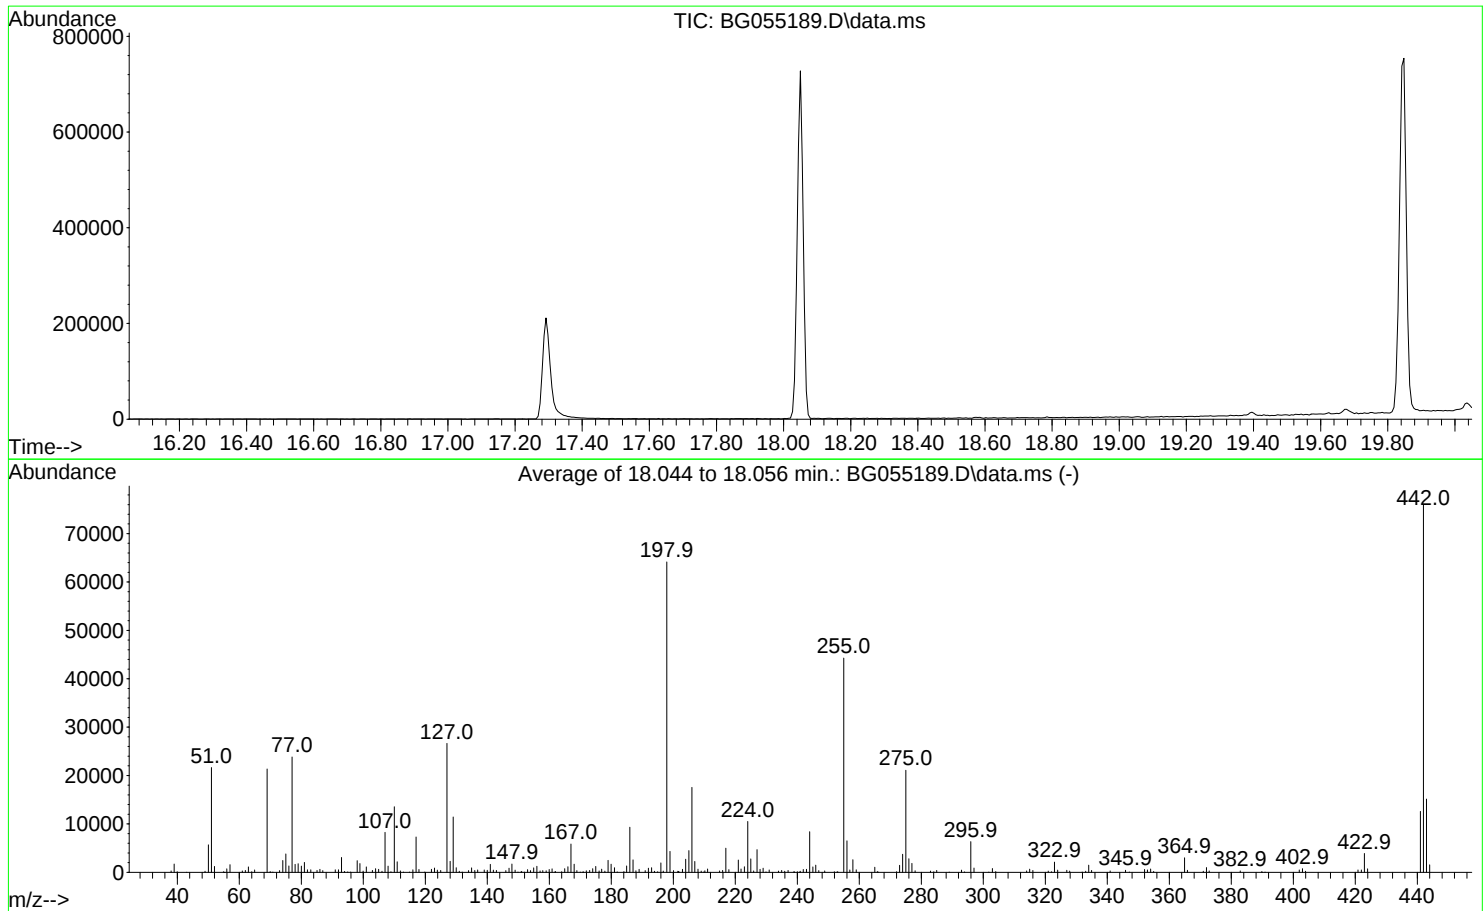




AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	21662	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.3	21361	PASS
70	69	0.00	2	0.4	88	PASS
127	198	10	80	41.5	26651	PASS
197	198	0.00	2	0.4	249	PASS
198	198	100	100	100.0	64149	PASS
199	198	5	9	6.8	4331	PASS
275	198	10	60	32.9	21096	PASS
365	198	1	100	4.7	2999	PASS
441	198	0.01	100	19.6	12582	PASS
442	442	50	100	100.0	76037	PASS
443	442	15	24	19.9	15124	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101722\  
Data File : BG055189.D  
Acq On    : 17 Oct 2022  10:38  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 17 17:40:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 13 05:14:13 2022
Response via : Initial Calibration

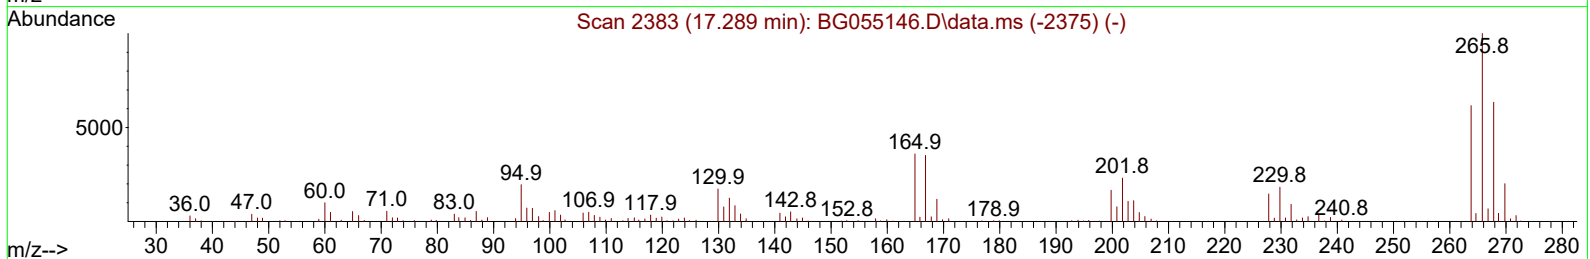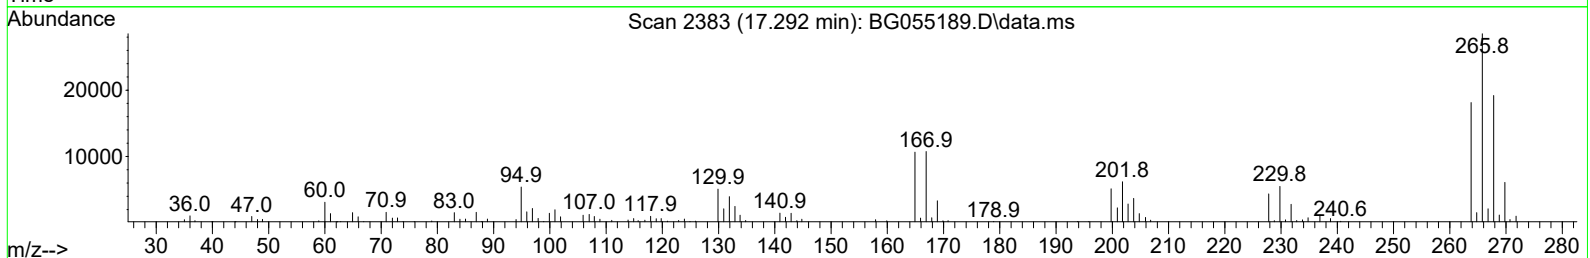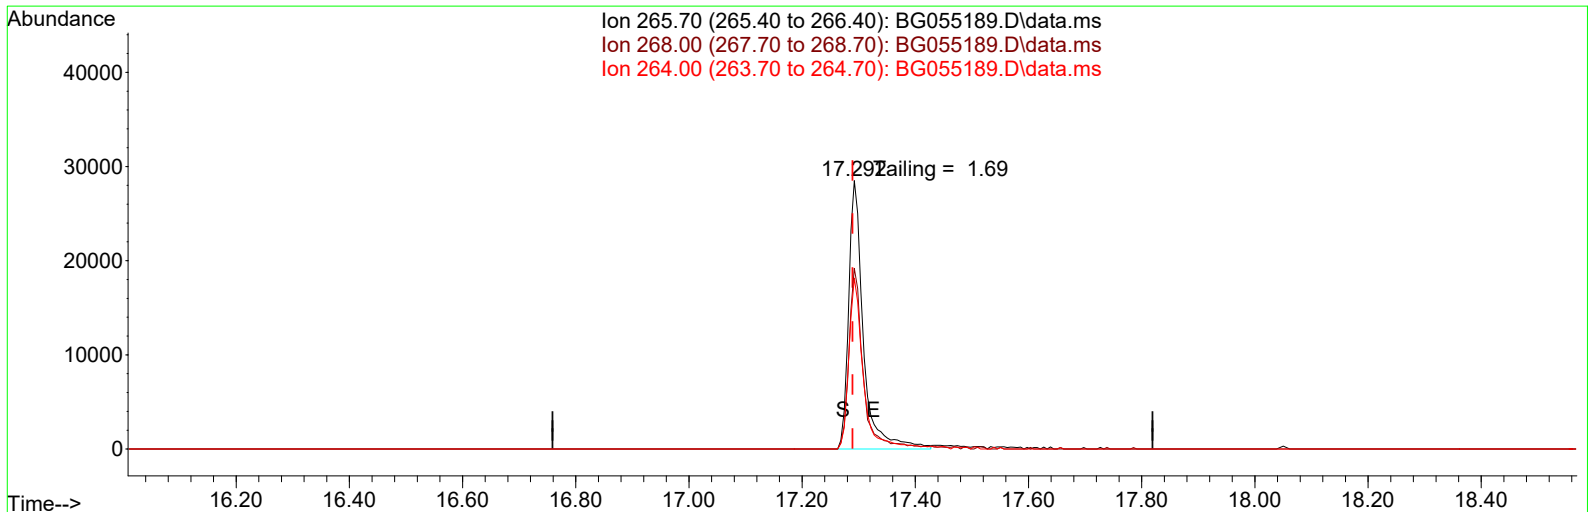

TIC: BG055189.D\data.ms

(70) Pentachlorophenol (C)

17.292min (+ 0.003) 21609.97 ng




response 51623

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.80	67.30
264.00	65.90	63.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101722\
Data File : BG055189.D
Acq On : 17 Oct 2022 10:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 17 17:40:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 13 05:14:13 2022
Response via : Initial Calibration

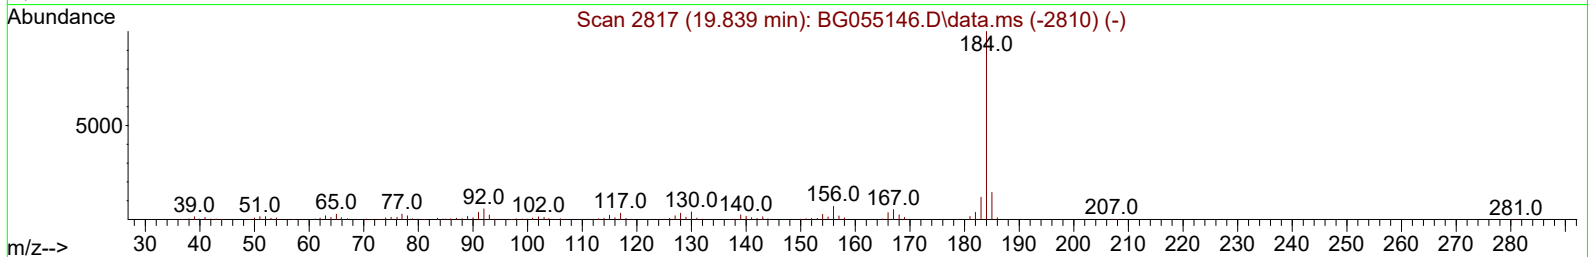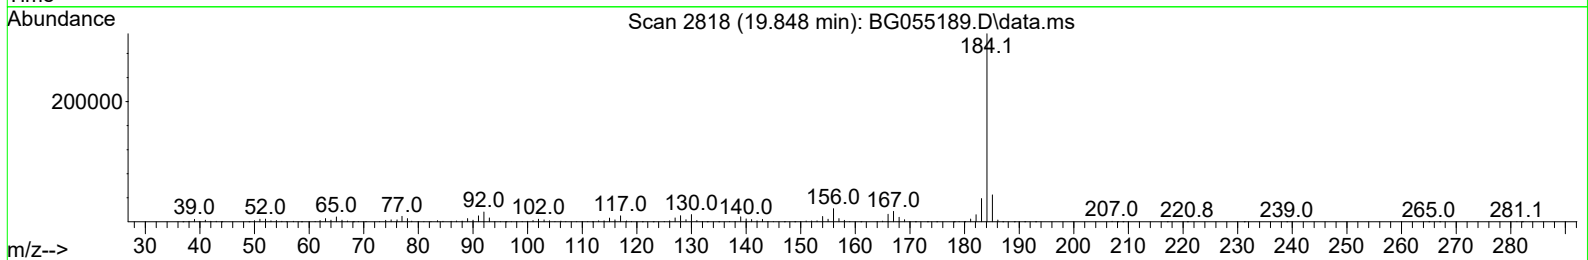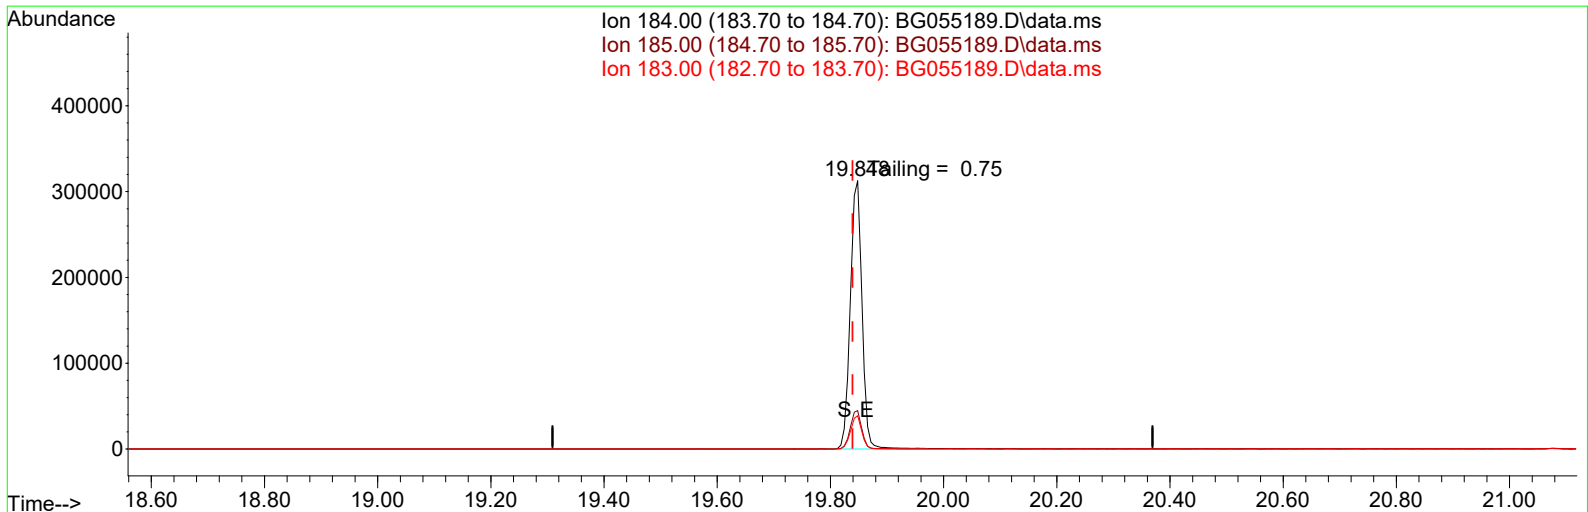

TIC: BG055189.D\data.ms

(77) Benzidine

19.848min (+ 0.009) 358316.13 ng

response 449977

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.31
183.00	11.80	12.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/17/2022	BNA_G	<u>BG055189.D</u>
Compound Name	Response	Retention Time
DDT	203413	21.076
DDD	4320	20.629
DDE	262	20.13
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4582	207995	2.20

Instrument :
BNA_G
ClientSampleId :
DFTPP