

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101817\
 Data File : BG029344.D
 Acq On : 18 Oct 2017 23:11
 Operator : SJ/JU
 Sample : I5834-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Oct 19 00:12:16 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 16 17:32:15 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	57760	20.00	ng	0.00
21) Naphthalene-d8	10.99	136	245666	20.00	ng	0.00
38) Acenaphthene-d10	14.78	164	162809	20.00	ng	-0.01
63) Phenanthrene-d10	17.52	188	423794	20.00	ng	0.00
75) Chrysene-d12	21.79	240	500540	20.00	ng	-0.01
86) Perylene-d12	25.10	264	504002	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.72	112	357257	103.33	ng	0.00
7) Phenol-d6	7.32	99	477151	98.32	ng	0.00
23) Nitrobenzene-d5	9.33	82	272530	70.50	ng	-0.01
41) 2,4,6-Tribromophenol	16.27	330	253328	120.52	ng	0.00
44) 2-Fluorobiphenyl	13.41	172	720009	64.86	ng	0.00
78) Terphenyl-d14	20.11	244	1278982	58.13	ng	-0.01
Target Compounds						
10) Phenol	7.34	94	29136	5.569	ng	94
40) Hexachlorocyclopentadiene	12.95	237	53	4.682	ng	# 22
49) Dimethylphthalate	14.22	163	186608	14.690	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101817\
Data File : BG029344.D
Acq On : 18 Oct 2017 23:11
Operator : SJ/JU
Sample : I5834-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Oct 19 00:12:16 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 16 17:32:15 2017
Response via : Initial Calibration

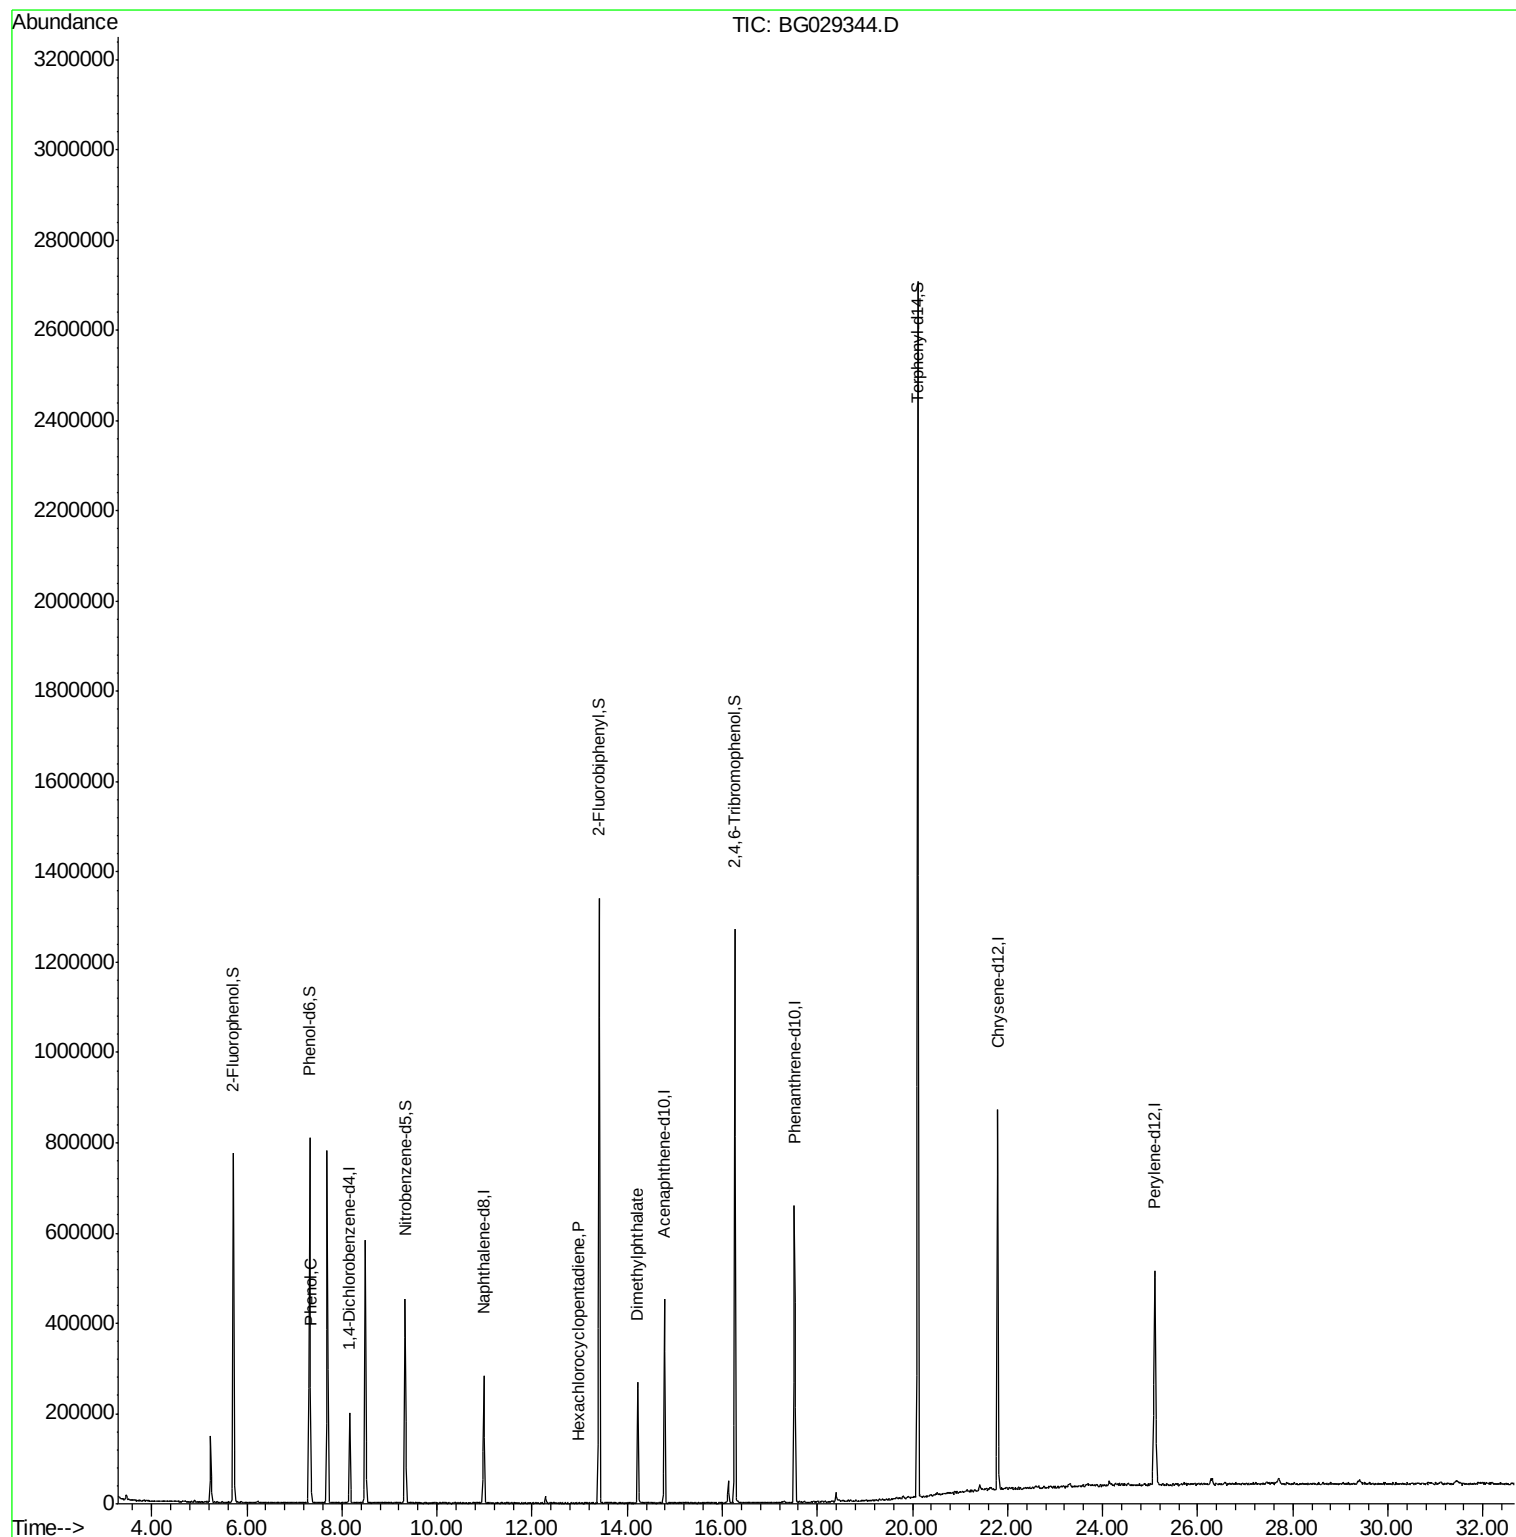

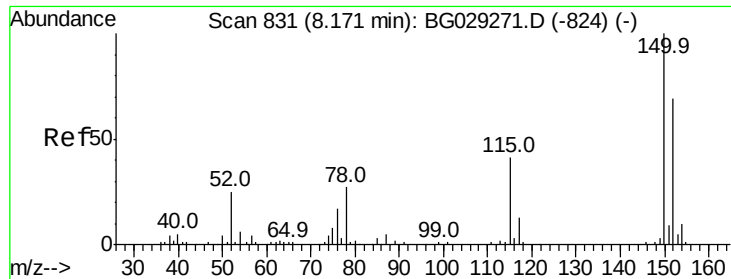


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.17 min Scan# 830
Delta R.T. -0.01 min
Lab File: BG029344.D
Acq: 18 Oct 2017 23:11

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 57760
Ion Ratio Lower Upper
152 100
150 153.3 126.6 189.8
115 54.9 53.0 79.4

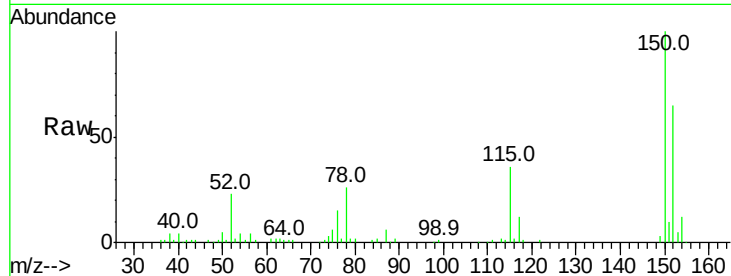


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

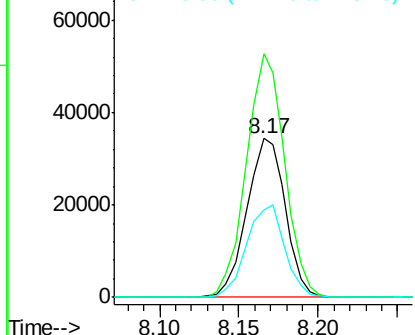



#5


2-Fluorophenol
Concen: 103.327 ng
RT: 5.72 min Scan# 414
Delta R.T. 0.00 min
Lab File: BG029344.D
Acq: 18 Oct 2017 23:11

Tgt Ion:112 Resp: 357257
Ion Ratio Lower Upper
112 100
64 60.1 56.3 84.5
63 30.9 30.1 45.1



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

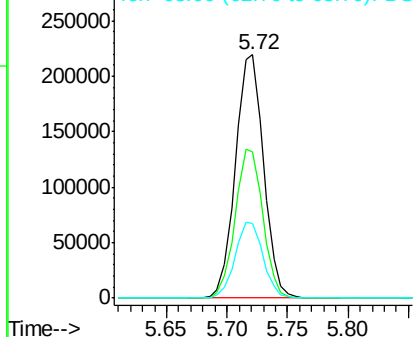

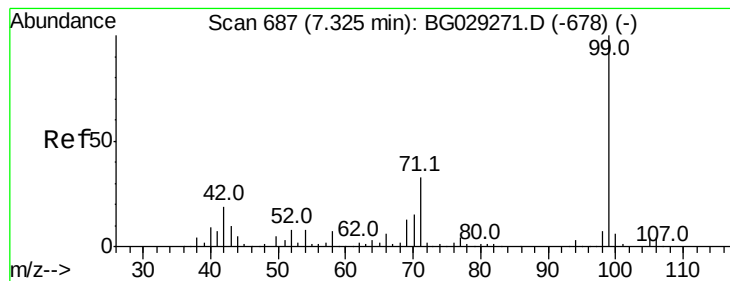

#7

Phenol-d6

Concen: 98.317 ng

RT: 7.32 min Scan# 686

Delta R.T. -0.01 min

Lab File: BG029344.D

Acq: 18 Oct 2017 23:11

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 477151

Ion Ratio Lower Upper




99 100

42 19.5 14.1 21.1

71 34.5 26.1 39.1

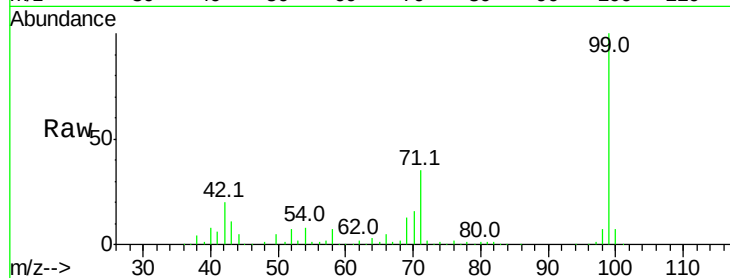

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

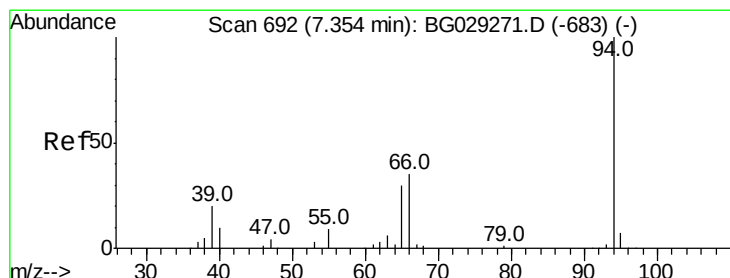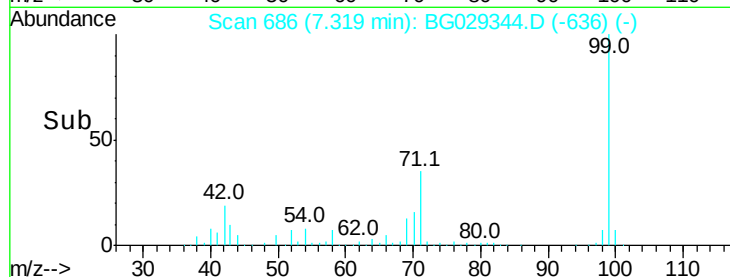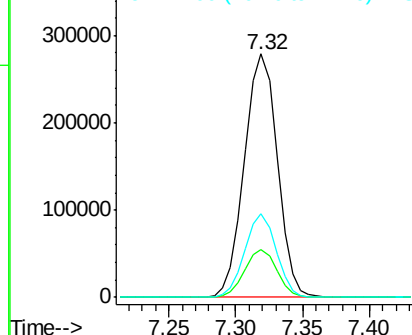

#10

Phenol

Concen: 5.569 ng

RT: 7.34 min Scan# 690

Delta R.T. -0.01 min

Lab File: BG029344.D

Acq: 18 Oct 2017 23:11


Tgt Ion: 94 Resp: 29136

Ion Ratio Lower Upper



94 100


65 30.4 11.9 51.9

66 37.2 22.2 62.2

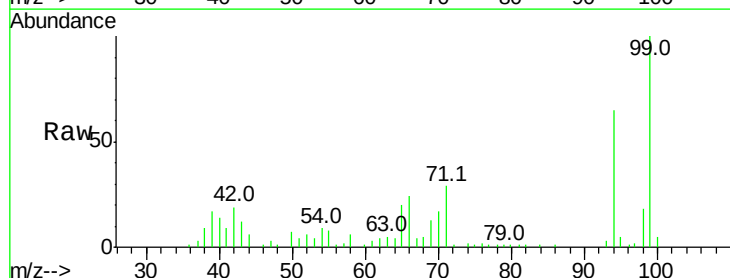

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

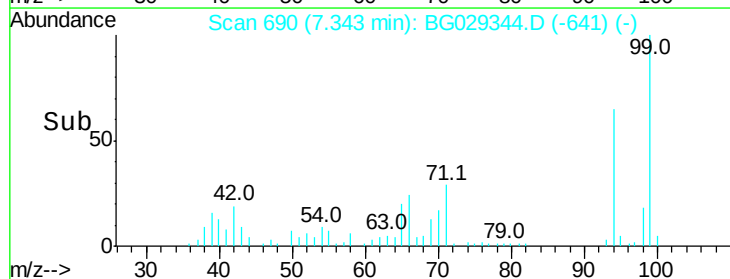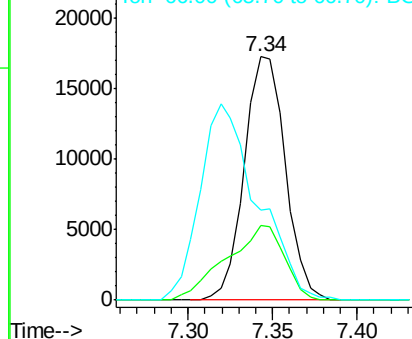







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.99 min Scan# 1310
Delta R.T. -0.01 min
Lab File: BG029344.D
Acq: 18 Oct 2017 23:11

Instrument :
BNA_G
ClientSampleId :

Tot Ion:136	Resp:	245666
Ion	Ratio	Lower Upper
136	100	
137	10.7	9.2 13.8
54	8.2	10.3 15.5#
68	6.0	4.5 6.7

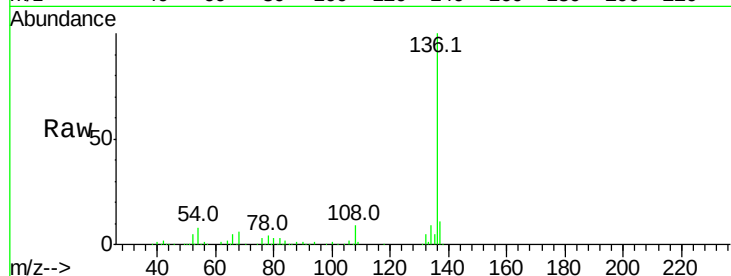


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


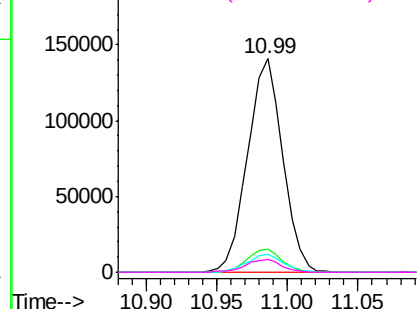



#23
Nitrobenzene-d5
Concen: 70.496 ng
RT: 9.33 min Scan# 1028
Delta R.T. -0.01 min
Lab File: BG029344.D
Acq: 18 Oct 2017 23:11

Tgt Ion: 82	Resp:	272530
Ion	Ratio	Lower Upper
82	100	
128	45.6	29.7 44.5#
54	53.7	43.1 64.7



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

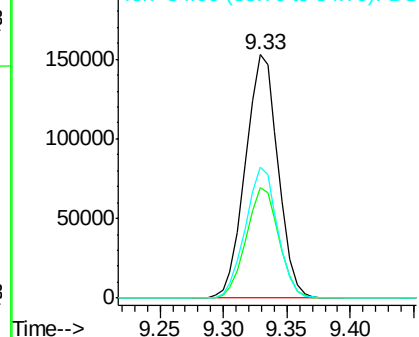



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.78 min Scan# 1956

Delta R.T. -0.01 min

Lab File: BG029344.D

Acq: 18 Oct 2017 23:11

Instrument :

BNA_G

ClientSampleId :


Tot Ion:164 Resp: 162809

Ion Ratio Lower Upper

164 100

162 102.2 78.8 118.2




160 44.0 35.4 53.0

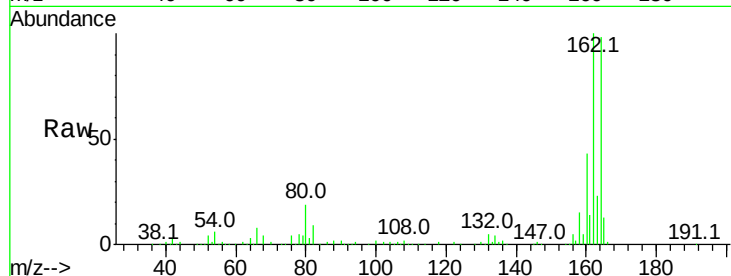

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

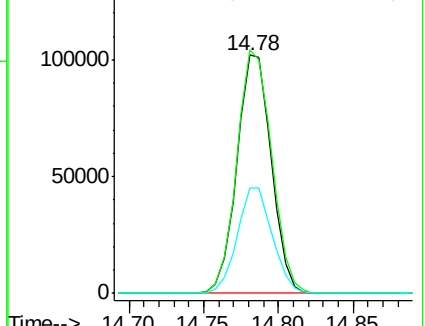

#40

Hexachlorocyclopentadiene

Concen: 4.682 ng

RT: 12.95 min Scan# 1645

Delta R.T. -0.02 min

Lab File: BG029344.D

Acq: 18 Oct 2017 23:11


Tgt Ion:237 Resp: 53

Ion Ratio Lower Upper

237 100

235 0.0 50.4 90.4#



272 0.0 0.0 31.8




Abundance Ion 236.80 (236.50 to 237.50): E

Ion 234.90 (234.60 to 235.60): E

Ion 271.75 (271.45 to 272.45): E

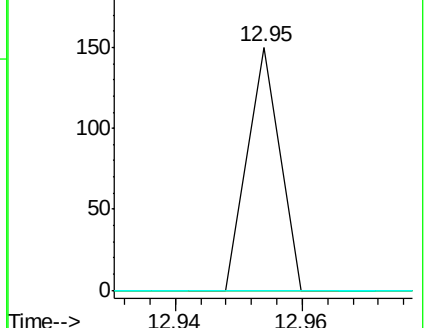


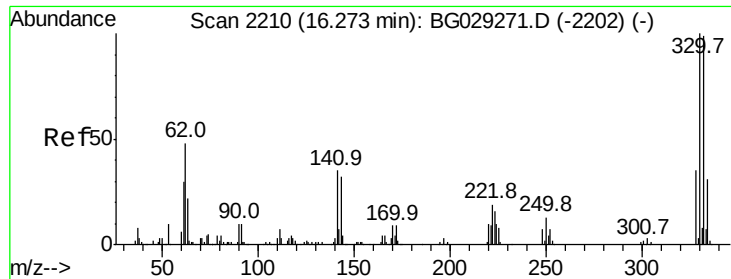




#41
 2,4,6-Tribromophenol
 Concen: 120.516 ng
 RT: 16.27 min Scan# 2209
 Delta R.T. -0.01 min
 Lab File: BG029344.D
 Acq: 18 Oct 2017 23:11

Instrument :
 BNA_G
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.9	77.0	115.6
141	32.9	25.2	37.8




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

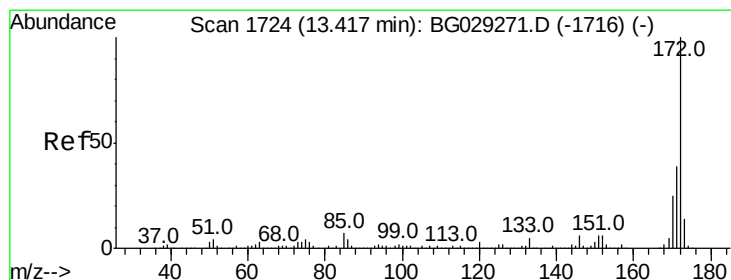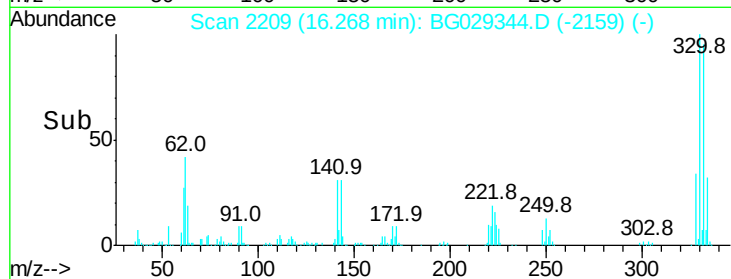
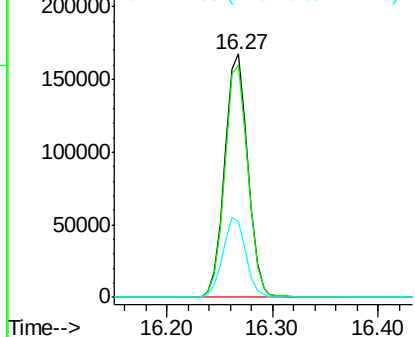



#44
 2-Fluorobiphenyl
 Concen: 64.862 ng
 RT: 13.41 min Scan# 1723
 Delta R.T. -0.01 min
 Lab File: BG029344.D
 Acq: 18 Oct 2017 23:11

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.6	30.0	45.0
170	23.9	19.5	29.3

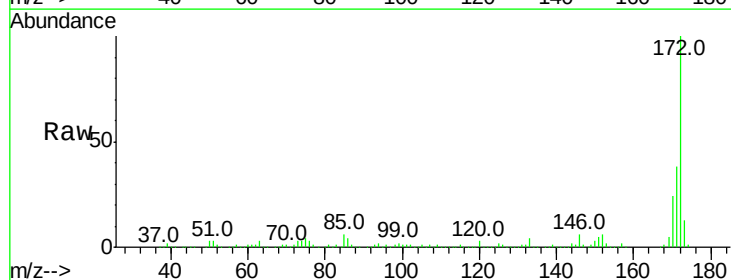

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

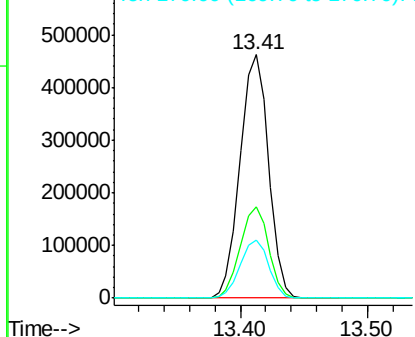

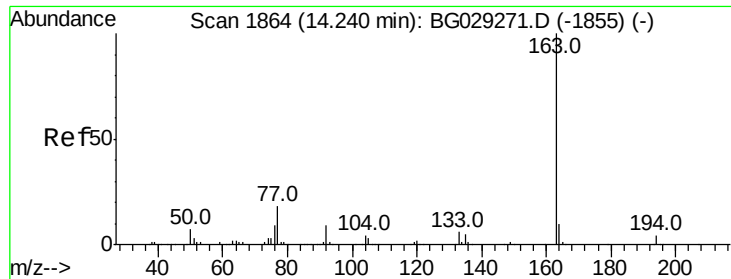

#49

Dimethylphthalate

Concen: 14.690 ng

RT: 14.22 min Scan# 1861

Delta R.T. -0.02 min

Lab File: BG029344.D

Acq: 18 Oct 2017 23:11

Instrument :

BNA_G

ClientSampleId :


Tot Ion:163 Resp: 186608

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.2




164 10.7 8.2 12.4



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

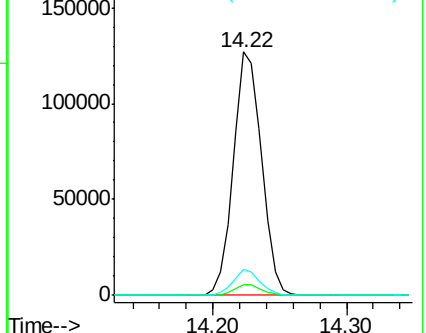

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.52 min Scan# 2423

Delta R.T. -0.01 min

Lab File: BG029344.D

Acq: 18 Oct 2017 23:11


Tgt Ion:188 Resp: 423794

Ion Ratio Lower Upper

188 100

94 7.5 6.9 10.3



80 9.1 7.7 11.5




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG0

Ion 80.00 (79.70 to 80.70): BG0

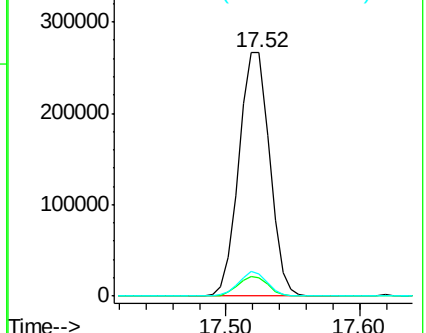

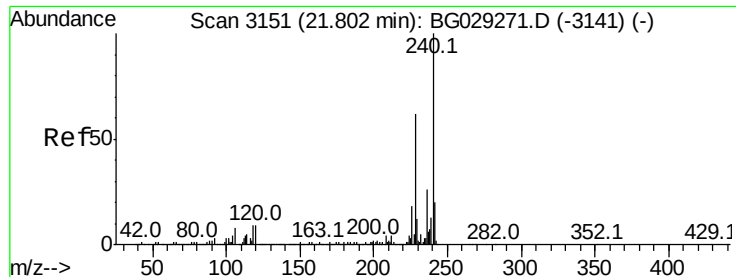

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.79 min Scan# 3149

Delta R.T. -0.01 min

Lab File: BG029344.D

Acq: 18 Oct 2017 23:11


Instrument :

BNA_G

ClientSampleId :

Tot Ion:240 Resp: 500540

Ion	Ratio	Lower	Upper
240	100		
120	9.8	6.8	10.2
236	27.1	20.9	31.3



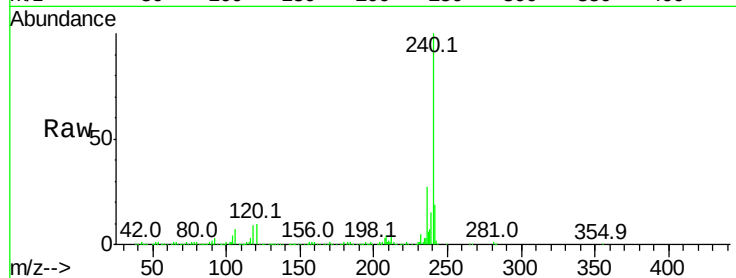


Abundance

Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

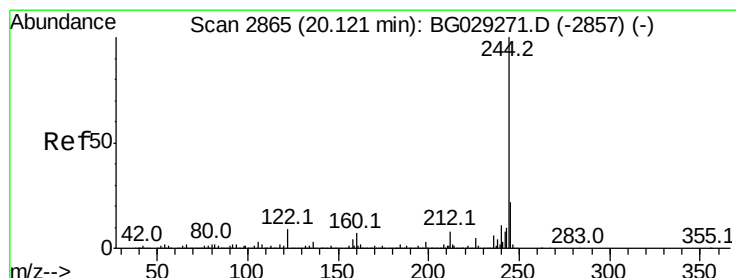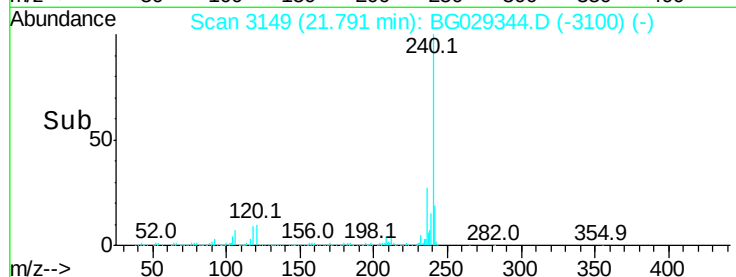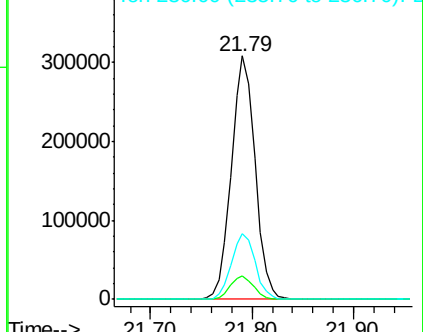

#78

Terphenyl-d14

Concen: 58.129 ng

RT: 20.11 min Scan# 2863


Delta R.T. -0.01 min

Lab File: BG029344.D

Acq: 18 Oct 2017 23:11

Tgt Ion:244 Resp: 1278982

Ion	Ratio	Lower	Upper
244	100		
212	7.7	5.8	8.8
122	9.4	7.0	10.4


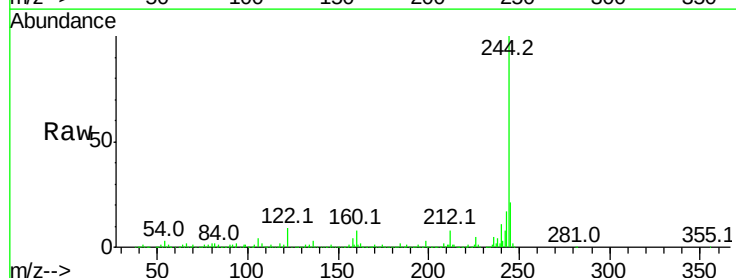





Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

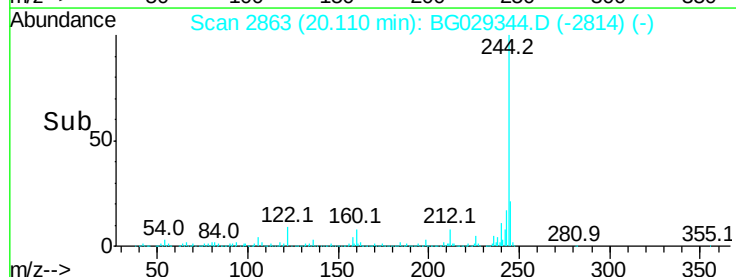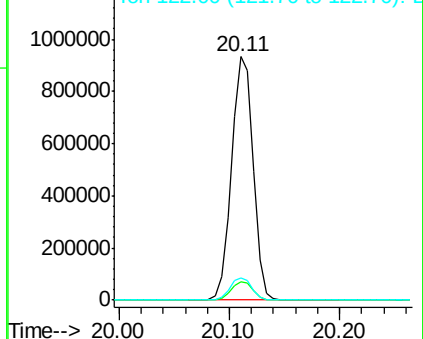

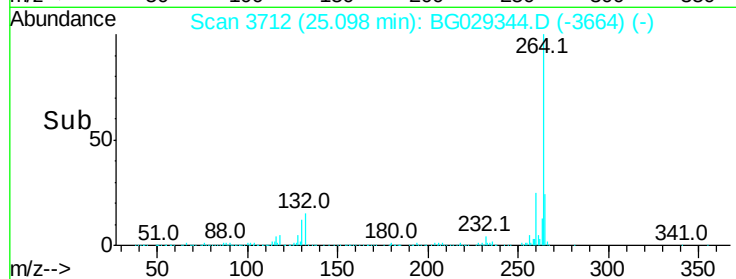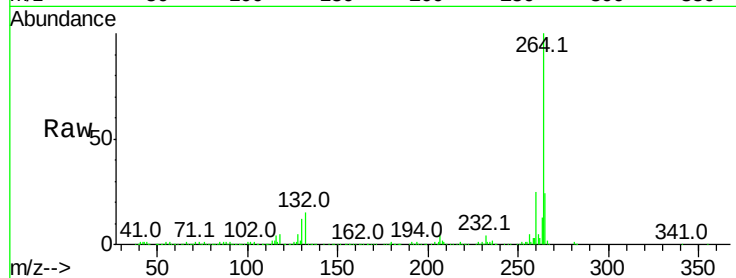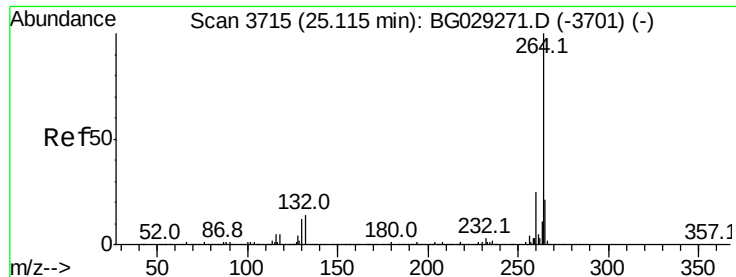

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 25.10 min Scan# 3712
 Delta R.T. -0.02 min
 Lab File: BG029344.D
 Acq: 18 Oct 2017 23:11

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	25.1	17.4	26.0
265	23.6	17.7	26.5

