

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101817\
 Data File : BG029353.D
 Acq On : 19 Oct 2017 5:08
 Operator : SJ/JU
 Sample : PB103395BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Oct 19 16:34:52 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 16 17:32:15 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	55095	20.00	ng	0.00
21) Naphthalene-d8	10.98	136	239336	20.00	ng	0.00
38) Acenaphthene-d10	14.79	164	156361	20.00	ng	0.00
63) Phenanthrene-d10	17.52	188	417091	20.00	ng	-0.01
75) Chrysene-d12	21.79	240	498764	20.00	ng	-0.01
86) Perylene-d12	25.10	264	506583	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.72	112	380186	115.28	ng	0.00
7) Phenol-d6	7.32	99	490473	105.95	ng	0.00
23) Nitrobenzene-d5	9.33	82	279275	74.15	ng	-0.01
41) 2,4,6-Tribromophenol	16.27	330	262527	130.04	ng	0.00
44) 2-Fluorobiphenyl	13.41	172	764572	71.72	ng	0.00
78) Terphenyl-d14	20.11	244	1499579	68.40	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101817\
Data File : BG029353.D
Acq On : 19 Oct 2017 5:08
Operator : SJ/JU
Sample : PB103395BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Oct 19 16:34:52 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 16 17:32:15 2017
Response via : Initial Calibration

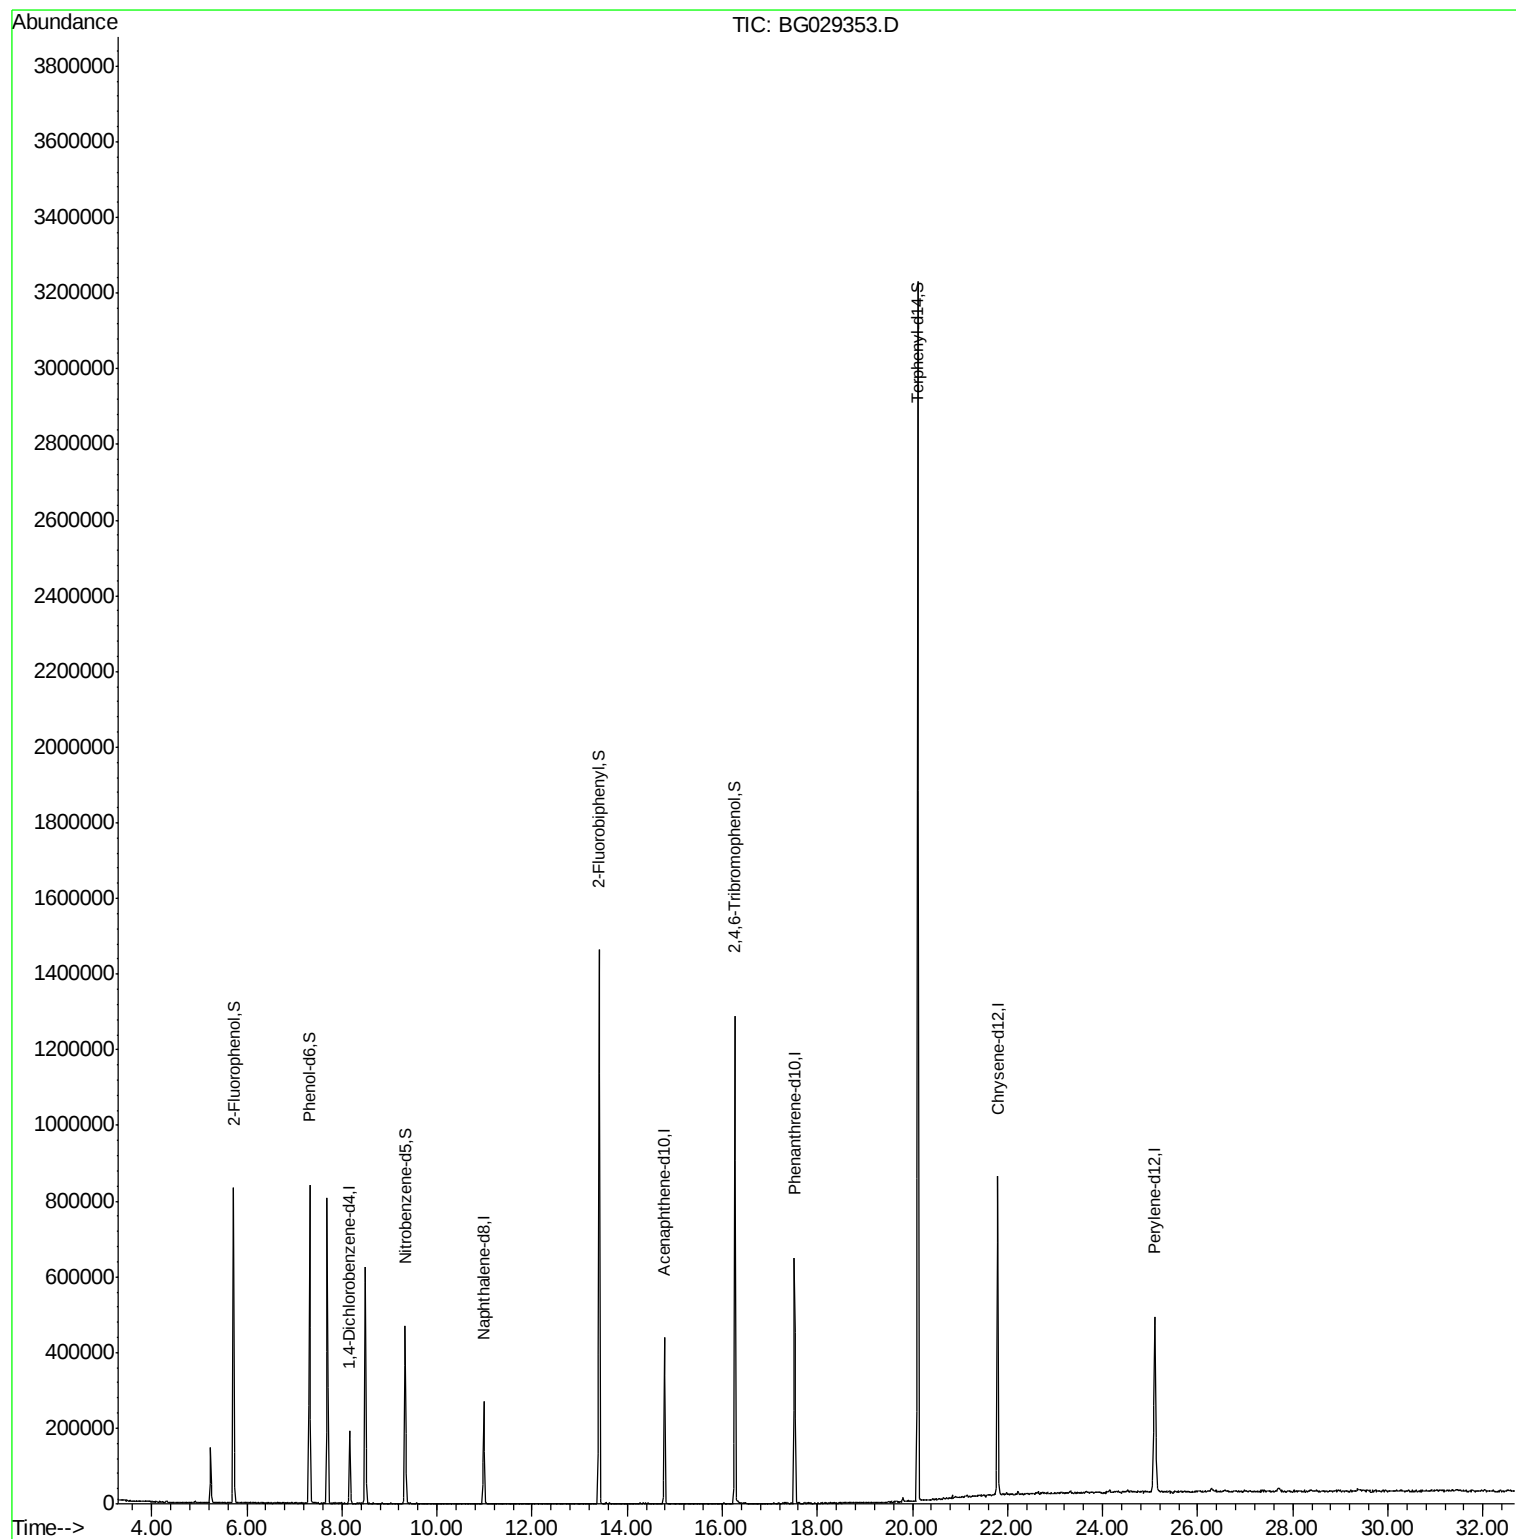




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.16 min Scan# 830
Delta R.T. -0.01 min
Lab File: BG029353.D
Acq: 19 Oct 2017 5:08

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 55095
Ion Ratio Lower Upper
152 100
150 150.3 126.6 189.8
115 59.8 53.0 79.4

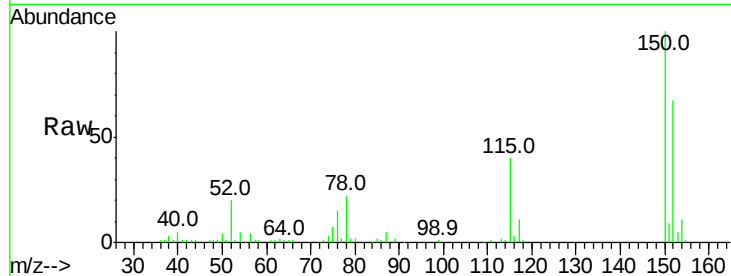


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

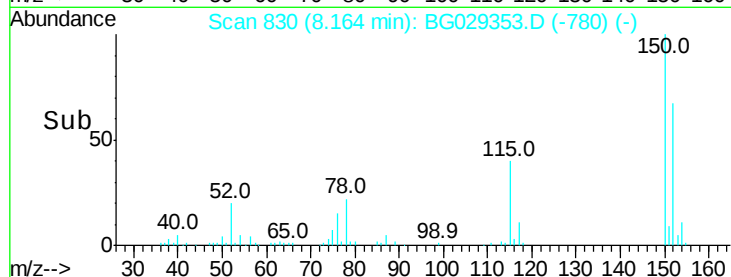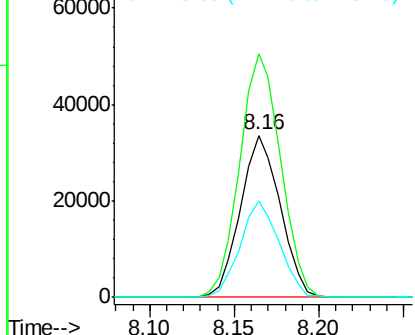



#5

2-Fluorophenol
Concen: 115.277 ng
RT: 5.72 min Scan# 414
Delta R.T. 0.00 min
Lab File: BG029353.D
Acq: 19 Oct 2017 5:08

Tgt Ion:112 Resp: 380186
Ion Ratio Lower Upper
112 100
64 59.5 56.3 84.5
63 30.3 30.1 45.1

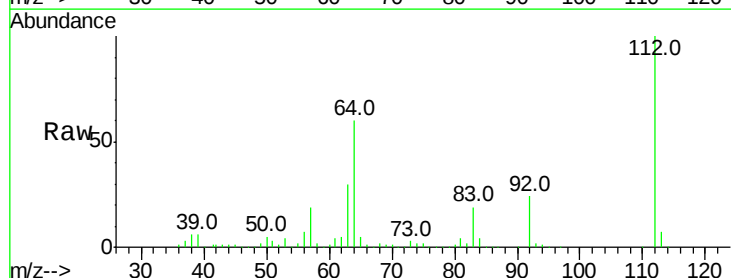

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

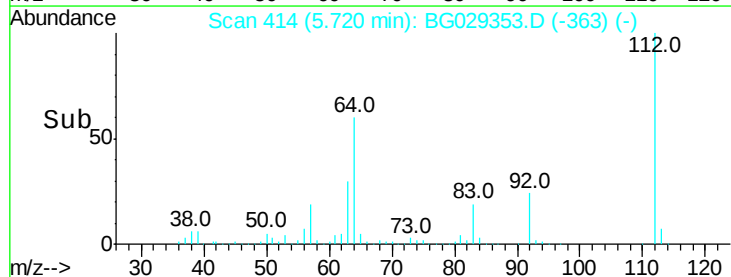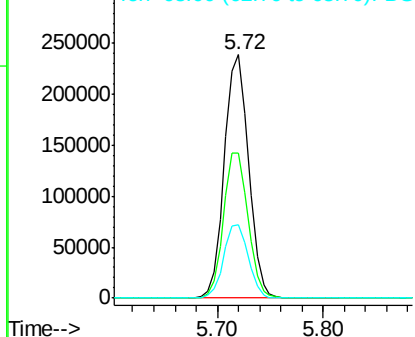



#7

Phenol-d6

Concen: 105.950 ng

RT: 7.32 min Scan# 686

Delta R.T. -0.01 min

Lab File: BG029353.D

Acq: 19 Oct 2017 5:08

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 490473

Ion Ratio Lower Upper




99 100

42 19.3 14.1 21.1

71 33.0 26.1 39.1

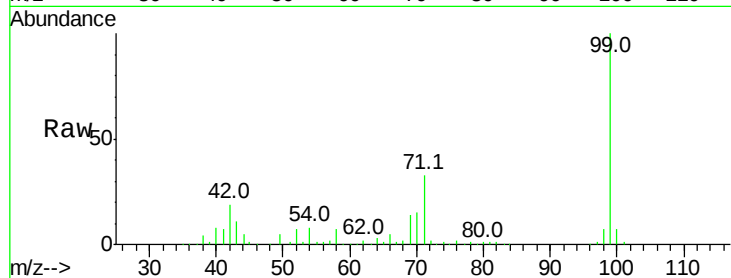

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

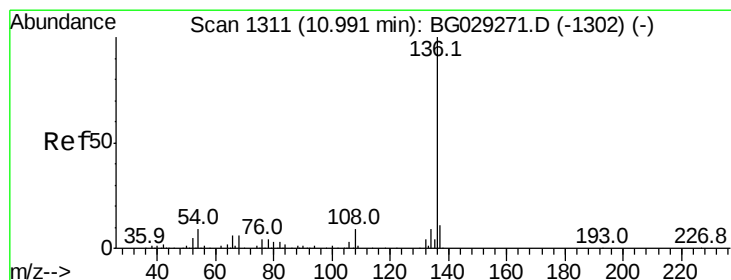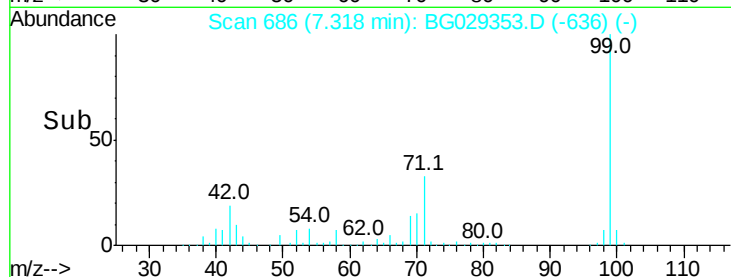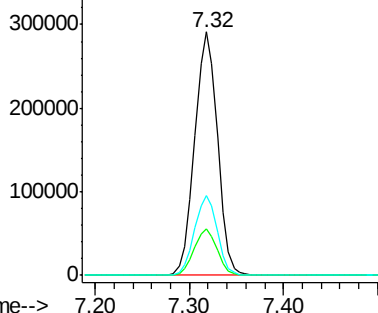

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.98 min Scan# 1310

Delta R.T. -0.01 min

Lab File: BG029353.D

Acq: 19 Oct 2017 5:08

Tgt Ion: 136 Resp: 239336


Ion Ratio Lower Upper

136 100



137 11.1 9.2 13.8


54 7.6 10.3 15.5#

68 5.4 4.5 6.7

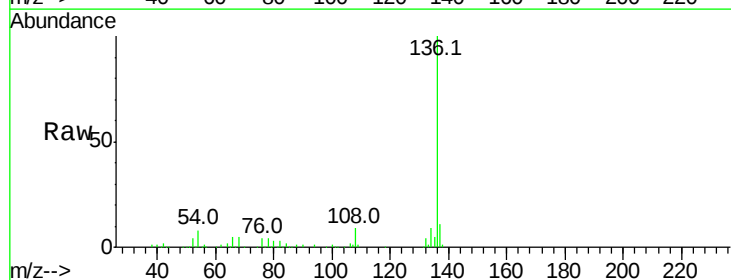

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



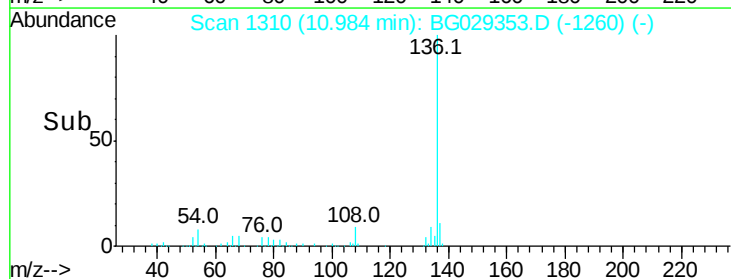
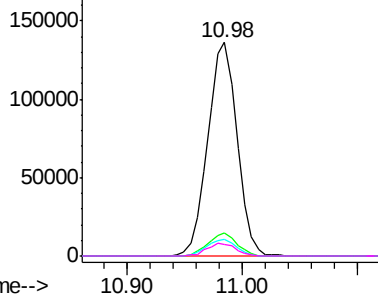


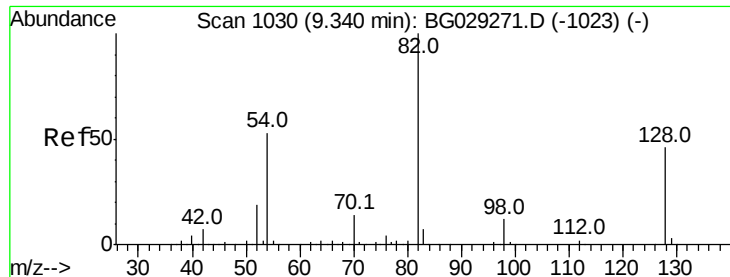

#23
 Nitrobenzene-d5
 Concen: 74.152 ng
 RT: 9.33 min Scan# 1028
 Delta R.T. -0.01 min
 Lab File: BG029353.D
 Acq: 19 Oct 2017 5:08




Instrument :
 BNA_G
 ClientSampled :


Tot Ion: 82 Resp: 279275
 Ion Ratio Lower Upper
 82 100
 128 45.4 29.7 44.5#
 54 51.0 43.1 64.7

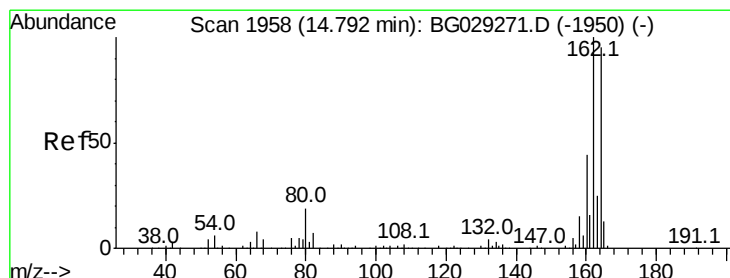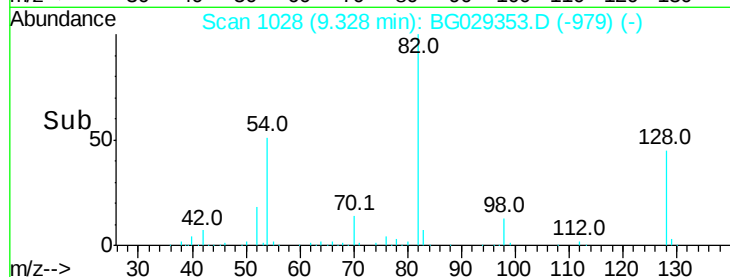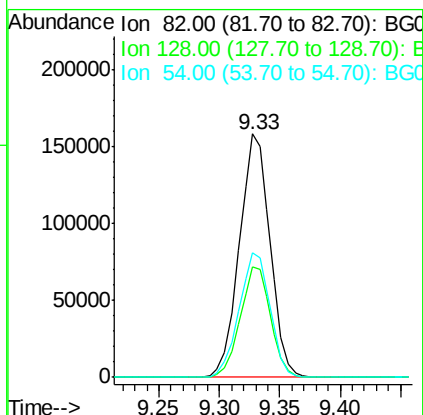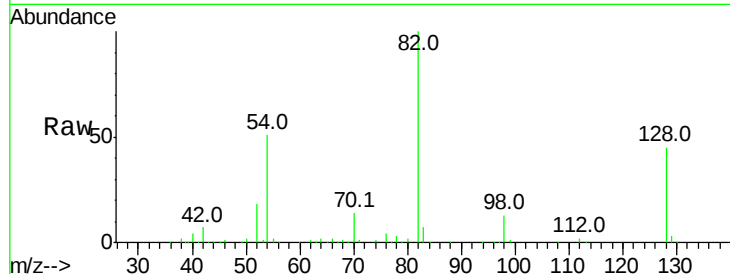

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.79 min Scan# 1957
 Delta R.T. -0.01 min
 Lab File: BG029353.D
 Acq: 19 Oct 2017 5:08

Tgt Ion: 164 Resp: 156361
 Ion Ratio Lower Upper
 164 100
 162 101.4 78.8 118.2
 160 44.2 35.4 53.0


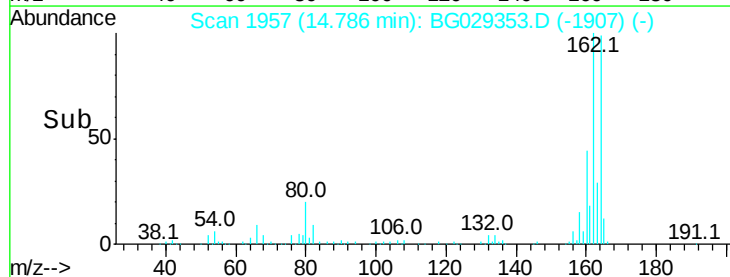
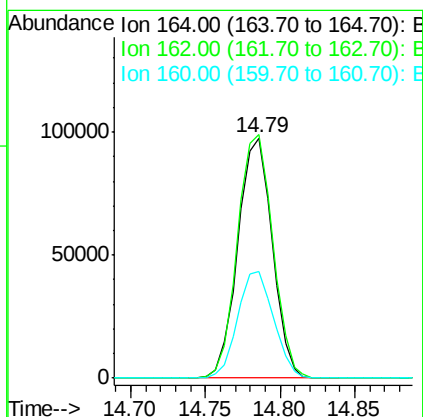
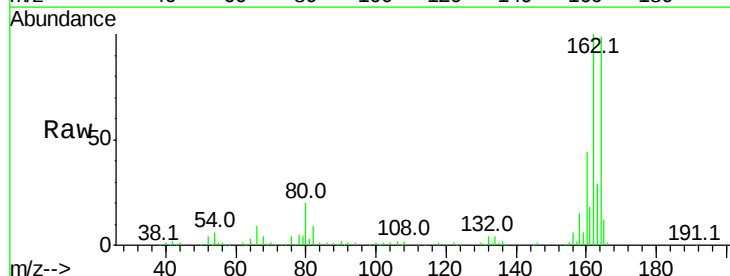


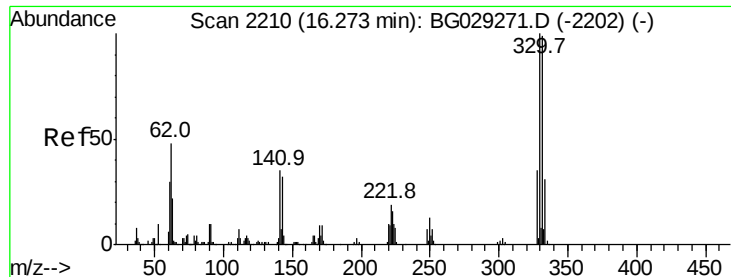

#41
 2,4,6-Tribromophenol
 Concen: 130.042 ng
 RT: 16.27 min Scan# 2209
 Delta R.T. -0.01 min
 Lab File: BG029353.D
 Acq: 19 Oct 2017 5:08




Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.5	77.0	115.6
141	33.1	25.2	37.8

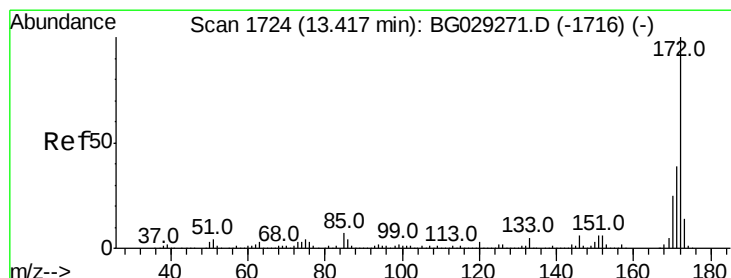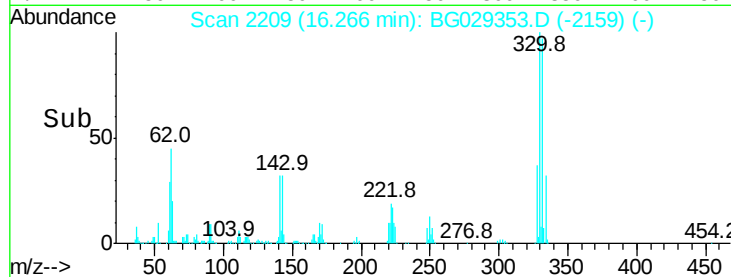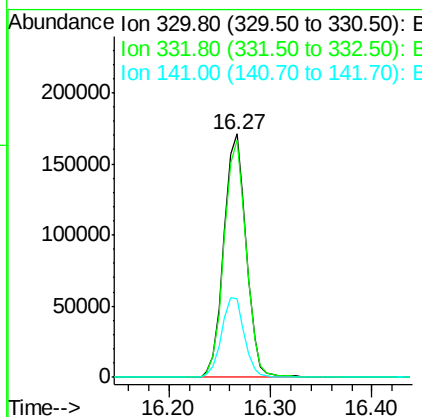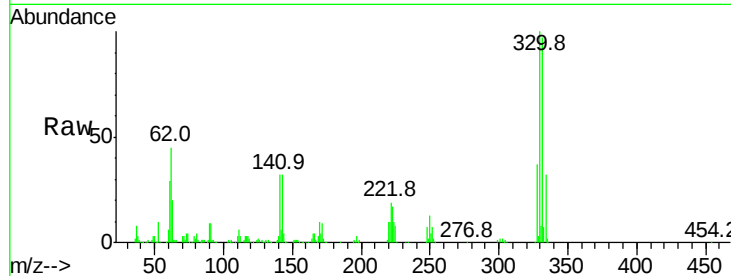

#44
 2-Fluorobiphenyl
 Concen: 71.716 ng
 RT: 13.41 min Scan# 1723
 Delta R.T. -0.01 min
 Lab File: BG029353.D
 Acq: 19 Oct 2017 5:08

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.9	30.0	45.0
170	24.0	19.5	29.3


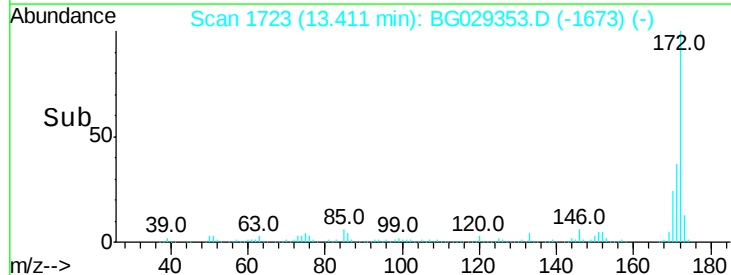
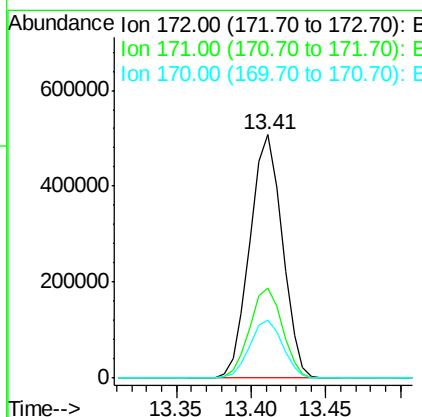
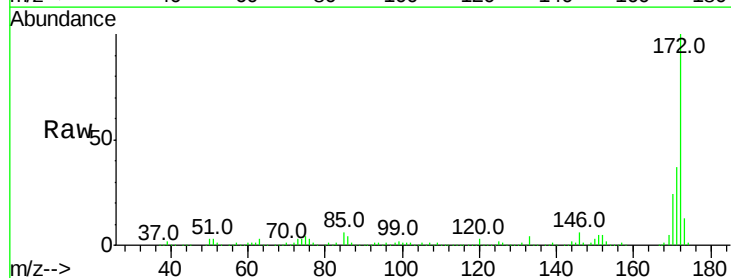




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.52 min Scan# 2422
Delta R.T. -0.01 min
Lab File: BG029353.D
Acq: 19 Oct 2017 5:08




Instrument :
BNA_G
ClientSampleId :

Tot Ion:188 Resp: 417091
Ion Ratio Lower Upper
188 100
94 8.0 6.9 10.3
80 10.0 7.7 11.5

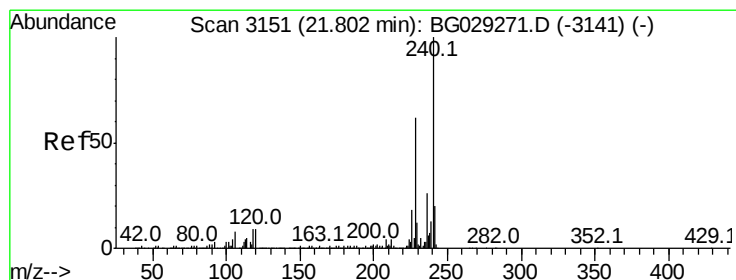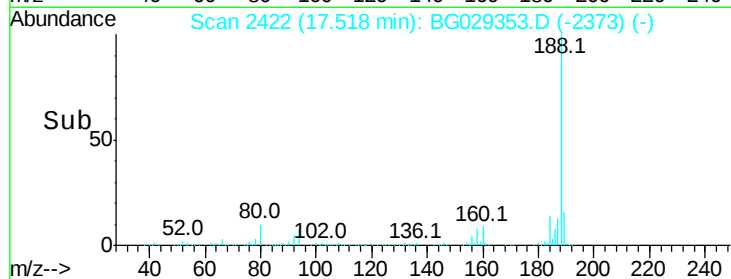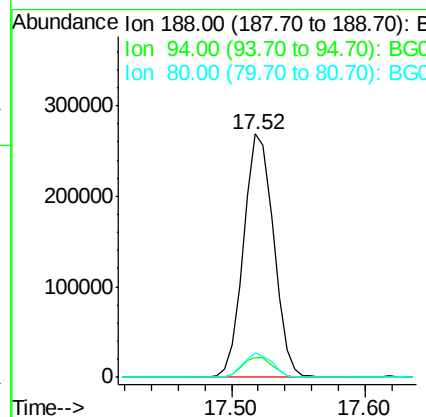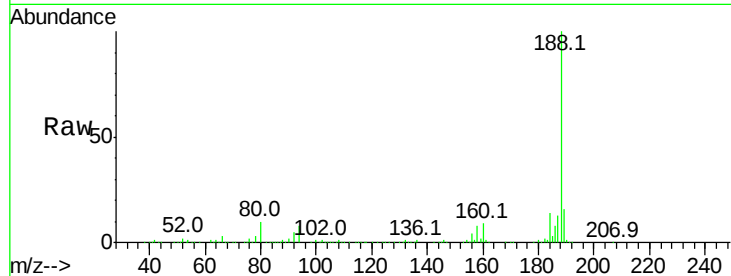

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.79 min Scan# 3149
Delta R.T. -0.01 min
Lab File: BG029353.D
Acq: 19 Oct 2017 5:08

Tgt Ion:240 Resp: 498764
Ion Ratio Lower Upper
240 100
120 9.7 6.8 10.2
236 26.0 20.9 31.3

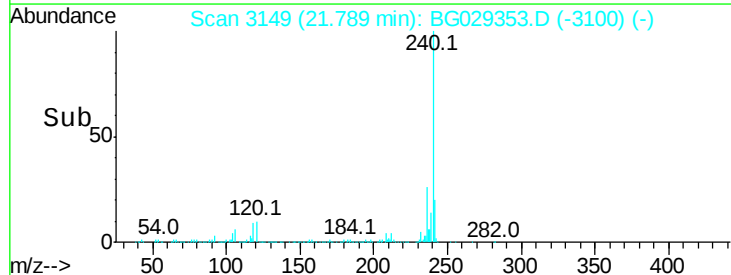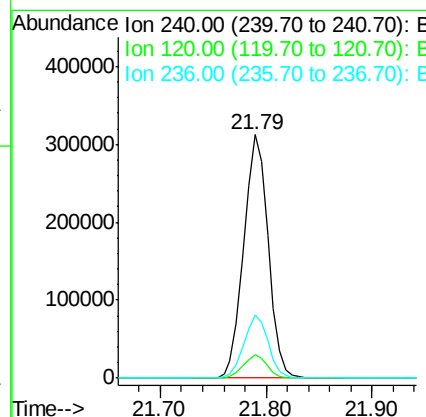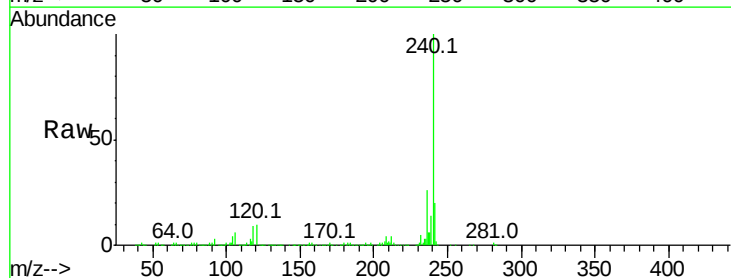



#78

Terphenyl-d14

Concen: 68.398 ng

RT: 20.11 min Scan# 2864

Delta R.T. -0.01 min

Lab File: BG029353.D

Acq: 19 Oct 2017 5:08





Instrument :

BNA_G

ClientSampled :

Tot Ion:244 Resp: 1499579

Ion	Ratio	Lower	Upper
244	100		
212	7.7	5.8	8.8
122	9.4	7.0	10.4

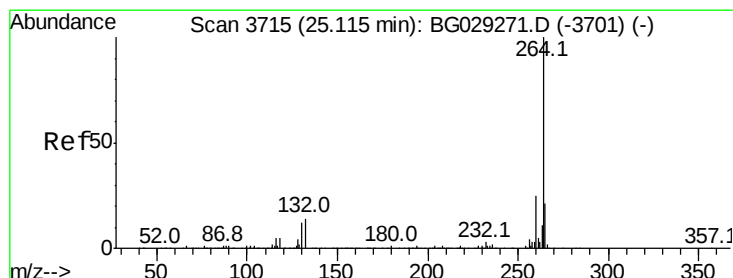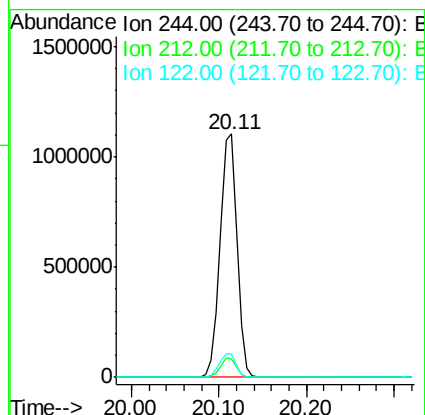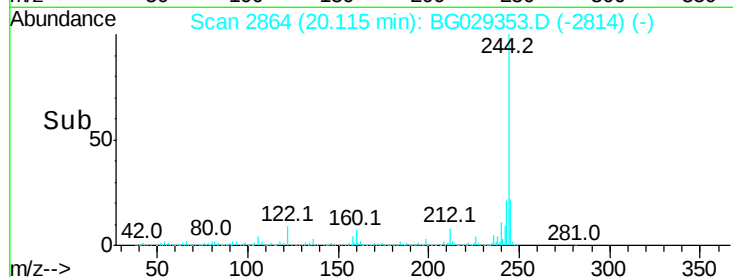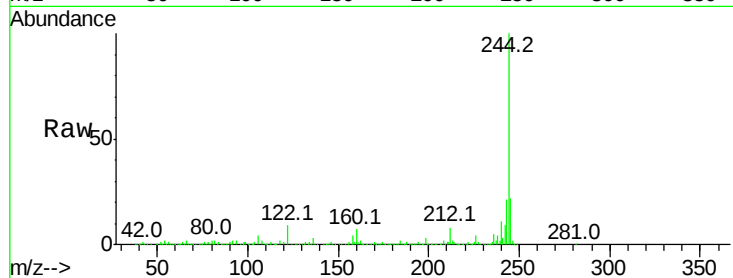

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.10 min Scan# 3712

Delta R.T. -0.02 min

Lab File: BG029353.D

Acq: 19 Oct 2017 5:08

Tgt Ion:264 Resp: 506583

Ion	Ratio	Lower	Upper
264	100		
260	23.5	17.4	26.0
265	21.1	17.7	26.5

