


Data Path : Z:\HPCHEM1\BNA G\Data\BG101817\
Data File : BG029355.D
Acq On : 19 Oct 2017 6:27
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG101617.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 16 17:32:15 2017

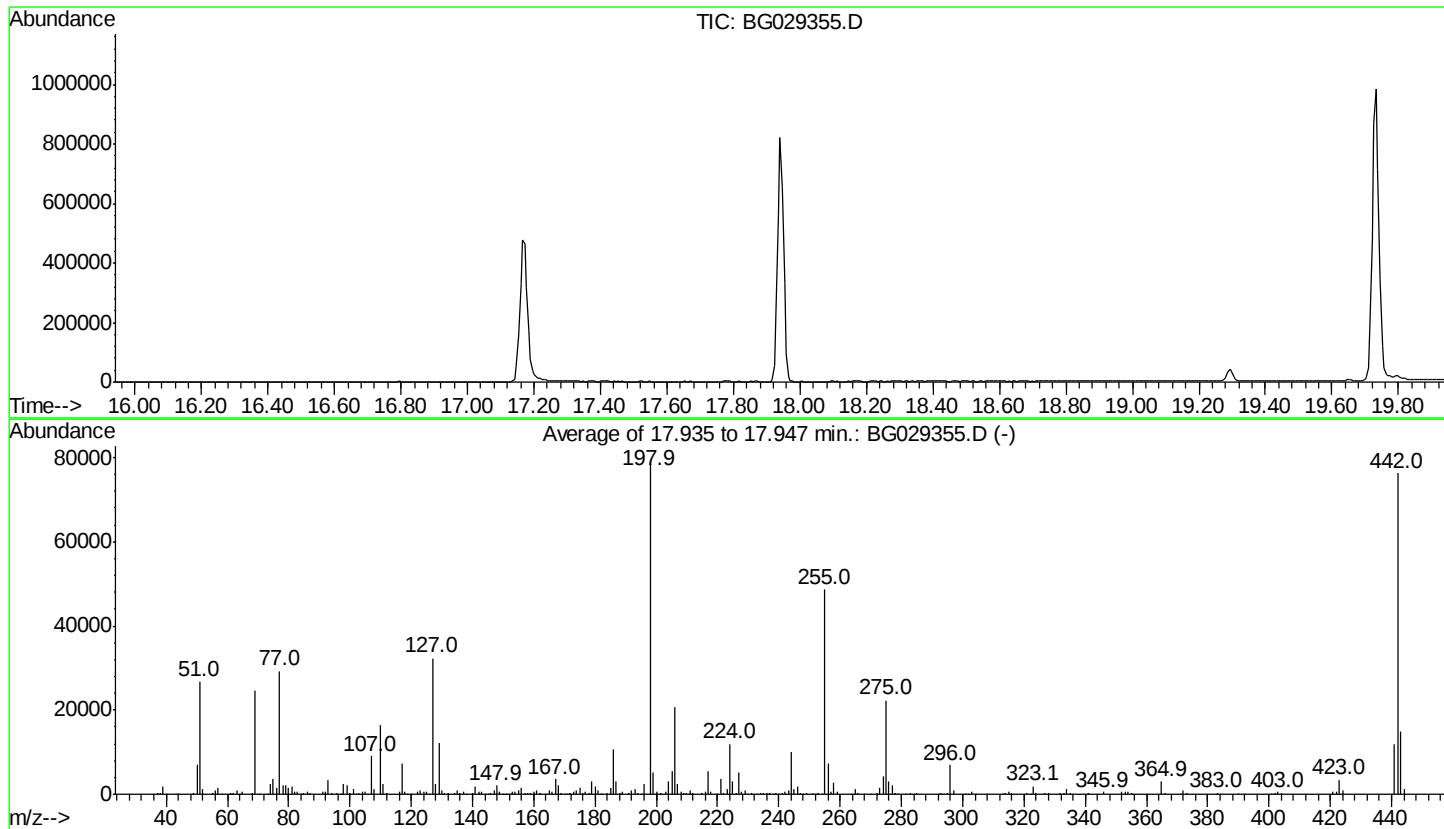

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	26725	PASS
68	69	0.00	2	1.2	289	PASS
69	198	0.00	100	31.5	24792	PASS
70	69	0.00	2	0.6	151	PASS
127	198	10	80	41.0	32274	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	78794	PASS
199	198	5	9	6.5	5148	PASS
275	198	10	60	28.3	22290	PASS
365	198	1	100	3.8	2971	PASS
441	442	0.01	24	15.7	11972	PASS
442	198	50	100	96.9	76322	PASS
443	442	15	24	19.7	15021	PASS