
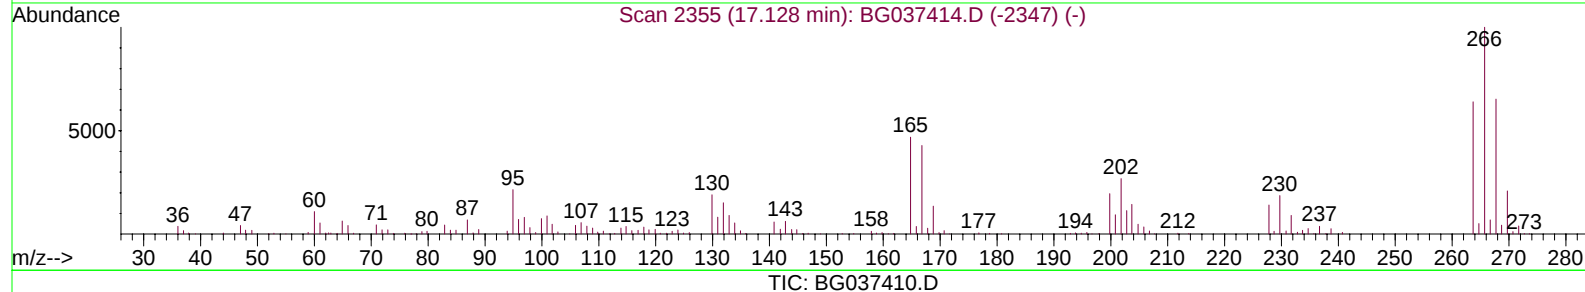
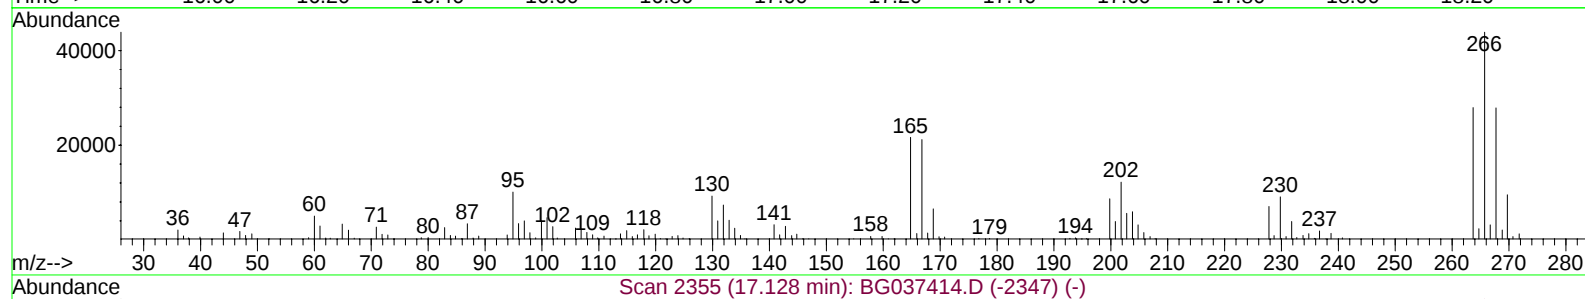


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101818\
Data File : BG037410.D
Acq On : 18 Oct 2018 8:35
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 19:03:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

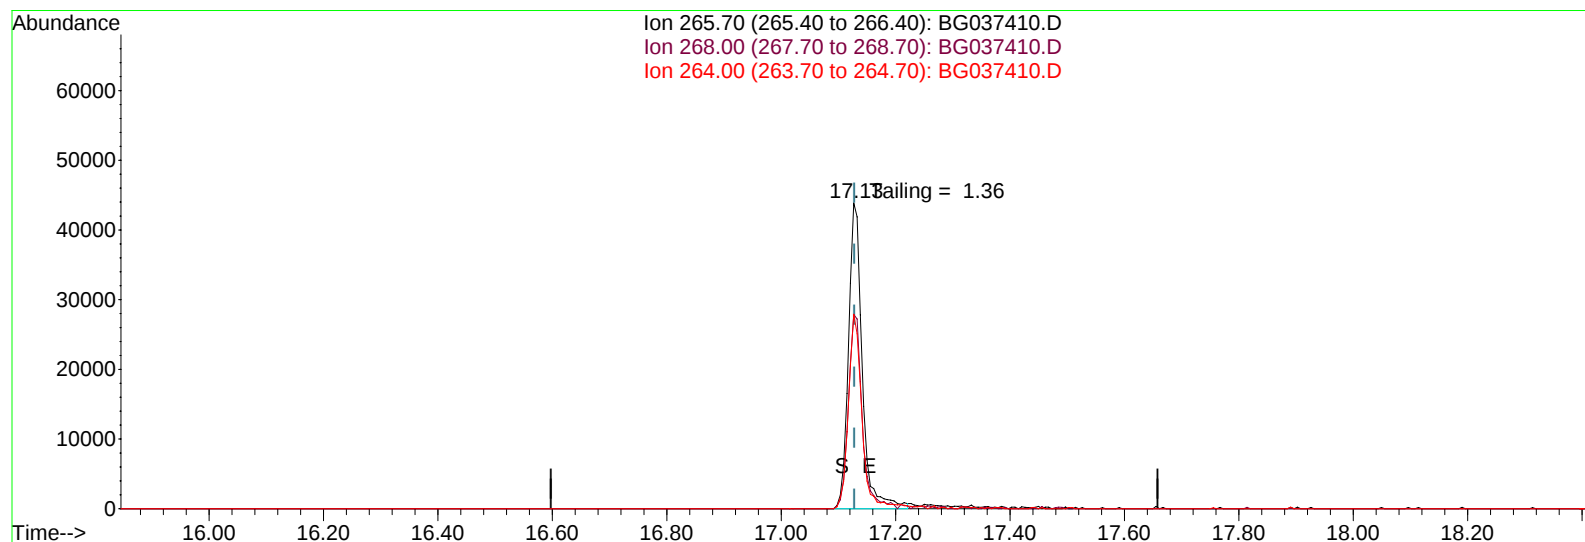

(70) Pentachlorophenol (C)




17.127min (-0.001) 42973.67ng

response 73714

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	63.53
264.00	73.60	68.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101818\
Data File : BG037410.D
Acq On : 18 Oct 2018 8:35
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 19:03:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

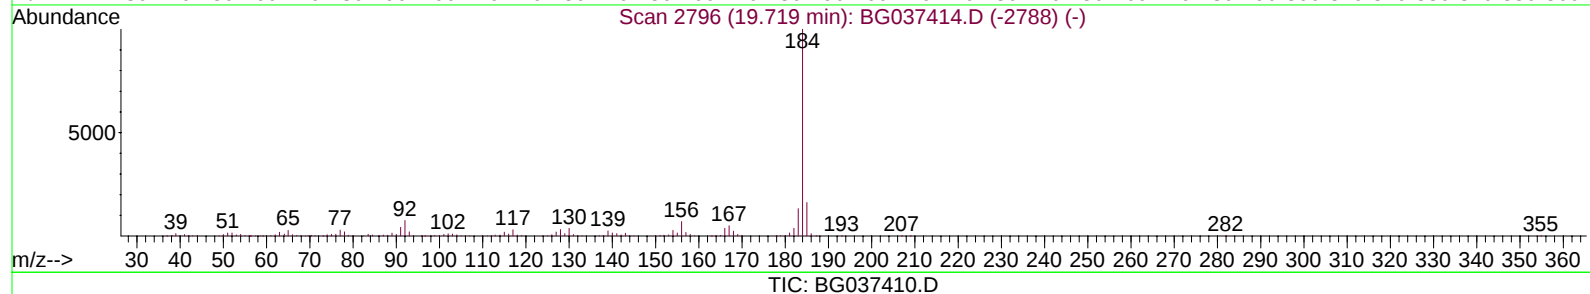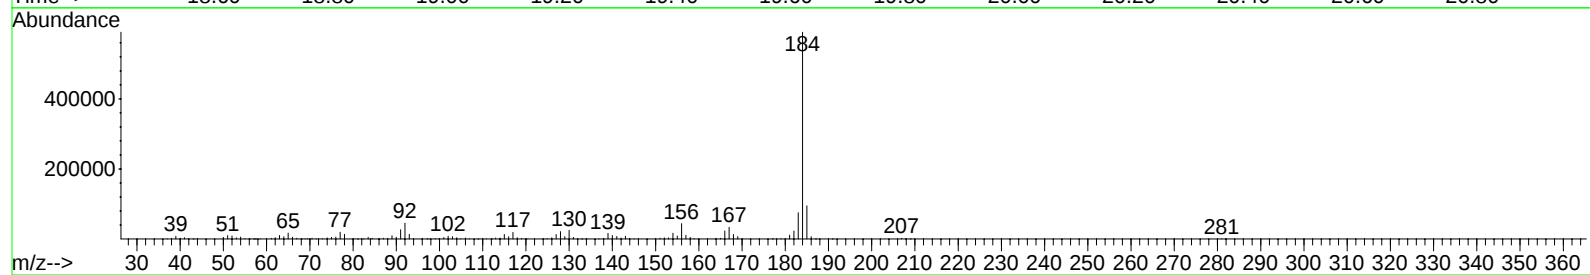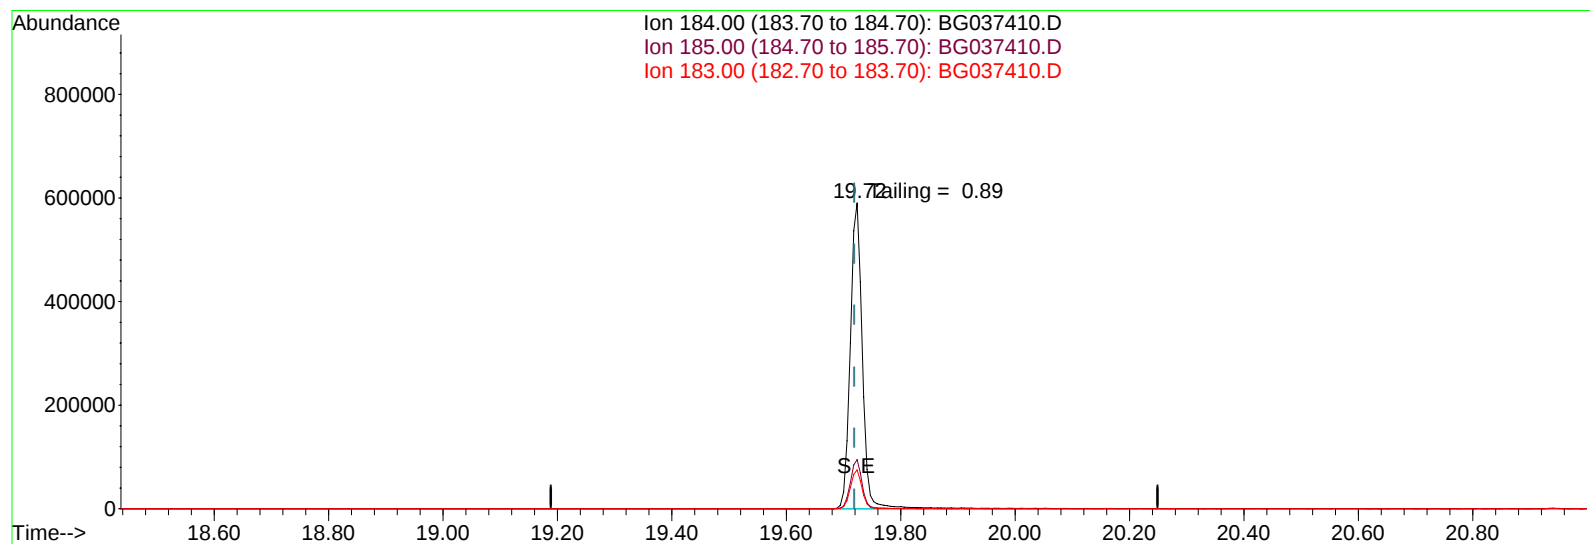

(77) Benzidine

19.724min (+0.005) 463926.57ng

response 867609

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.05
183.00	12.70	12.71
0.00	0.00	0.00