
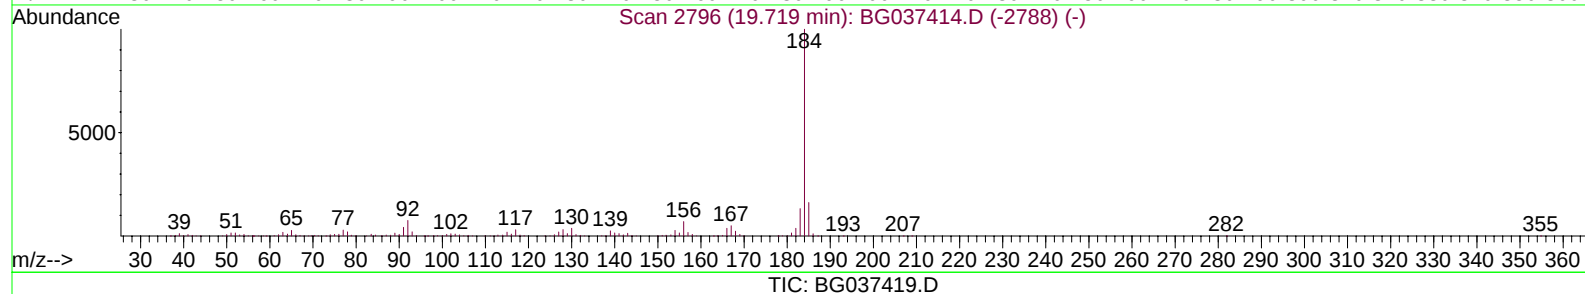
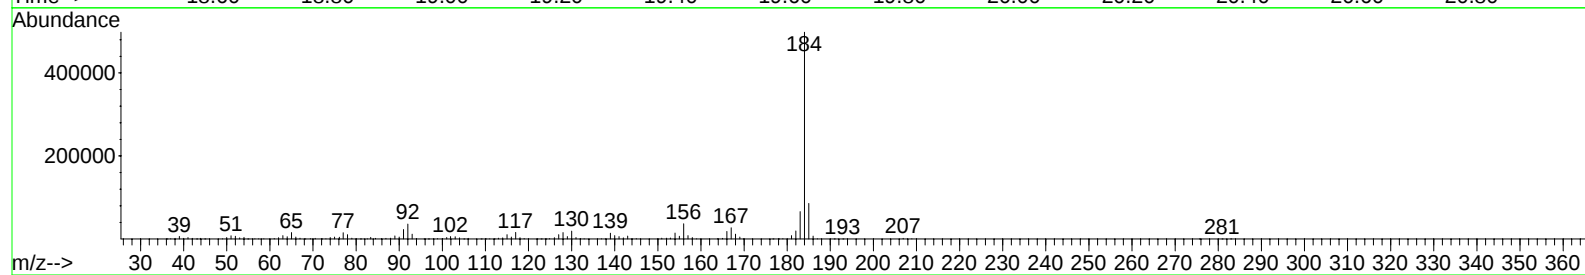


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101818\
Data File : BG037419.D
Acq On : 18 Oct 2018 14:44
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 11:05:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

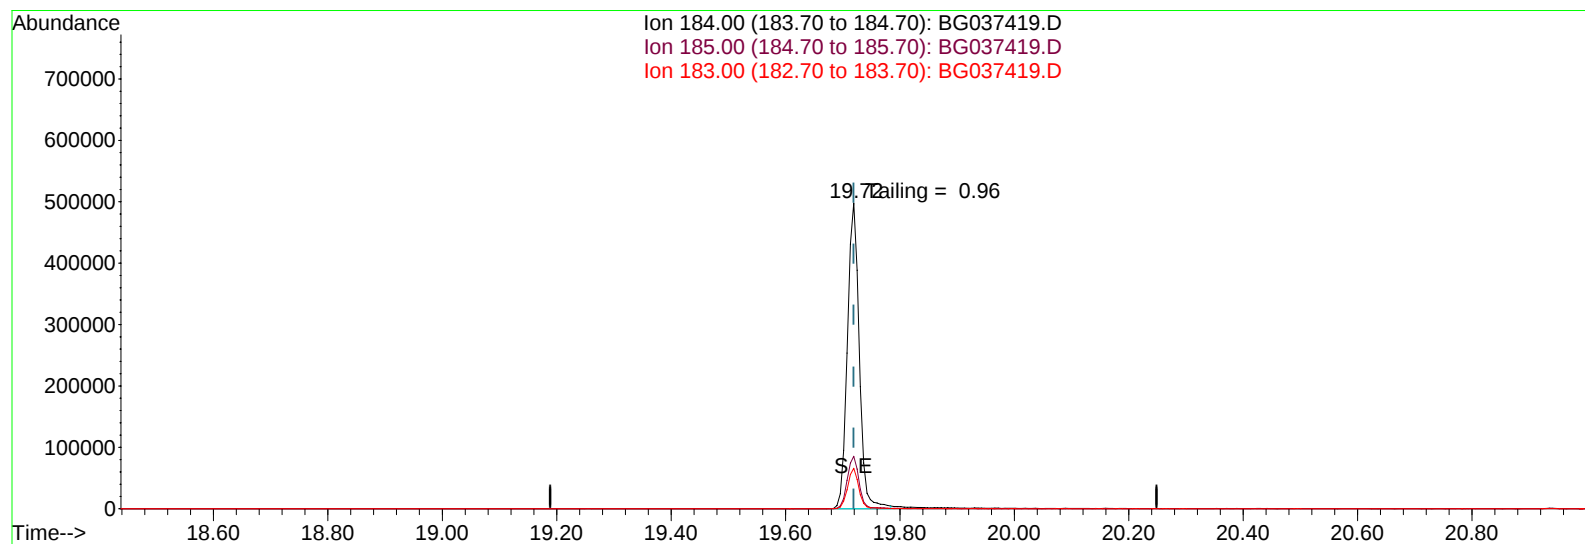

TIC: BG037419.D

(77) Benzidine




19.719min (+0.000) 0.00ng

response 734499

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	17.18
183.00	12.70	13.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101818\
Data File : BG037419.D
Acq On : 18 Oct 2018 14:44
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 11:05:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

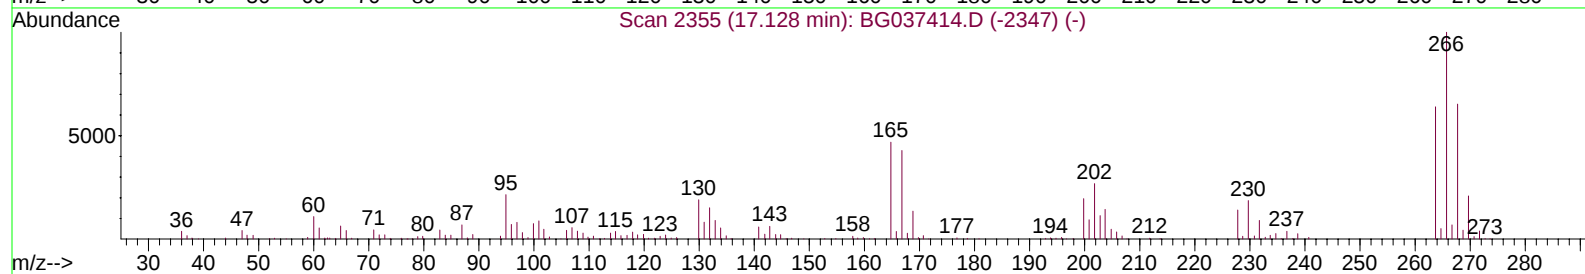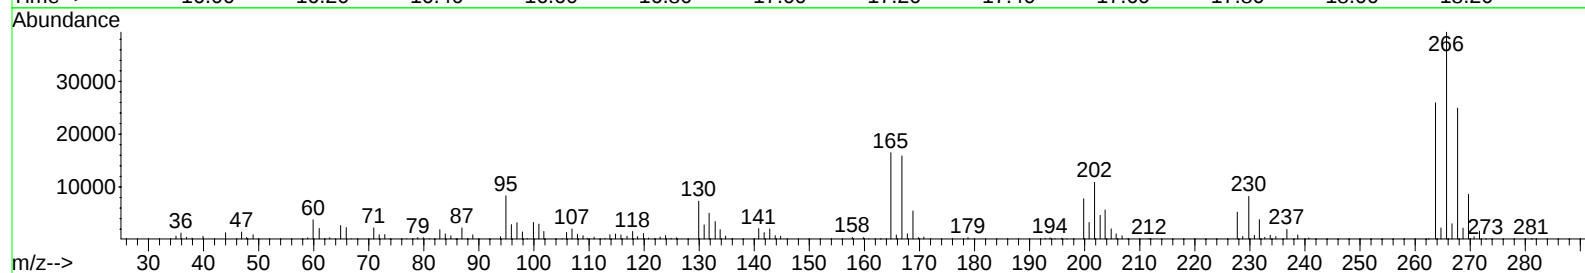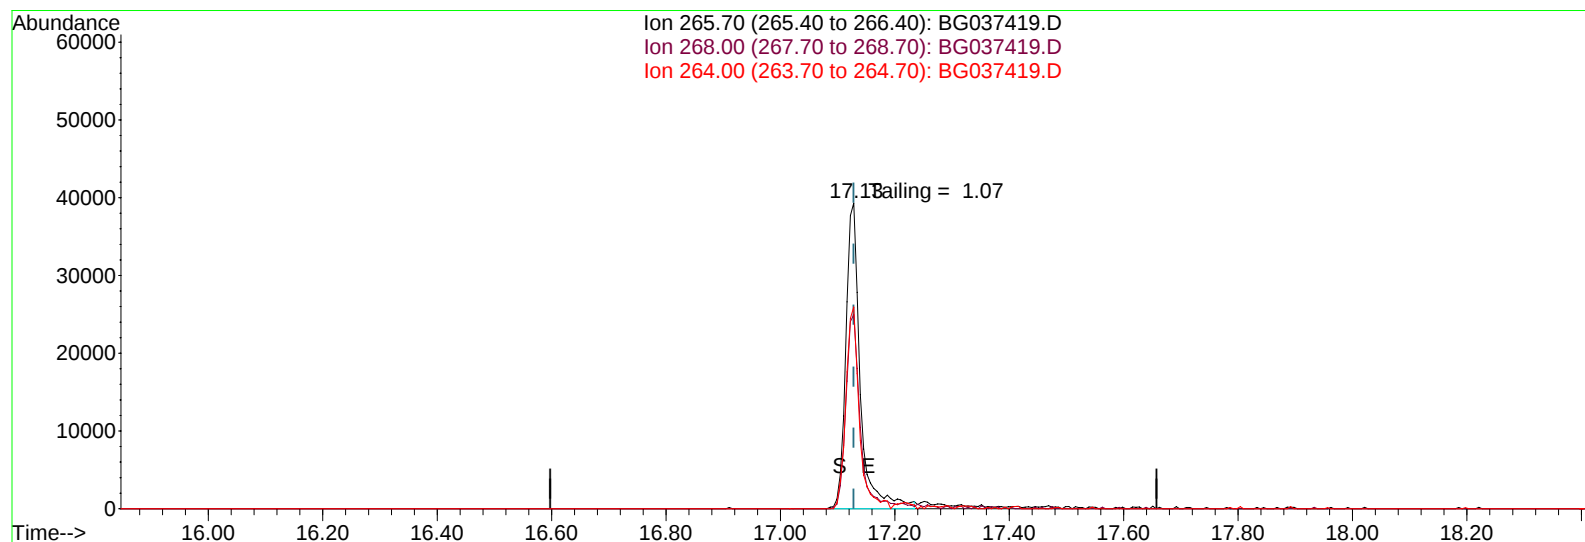

TIC: BG037419.D

(70) Pentachlorophenol (C)

17.128min (+0.000) 26675.13ng

response 68940

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	69.10
264.00	73.60	71.69
0.00	0.00	0.00