
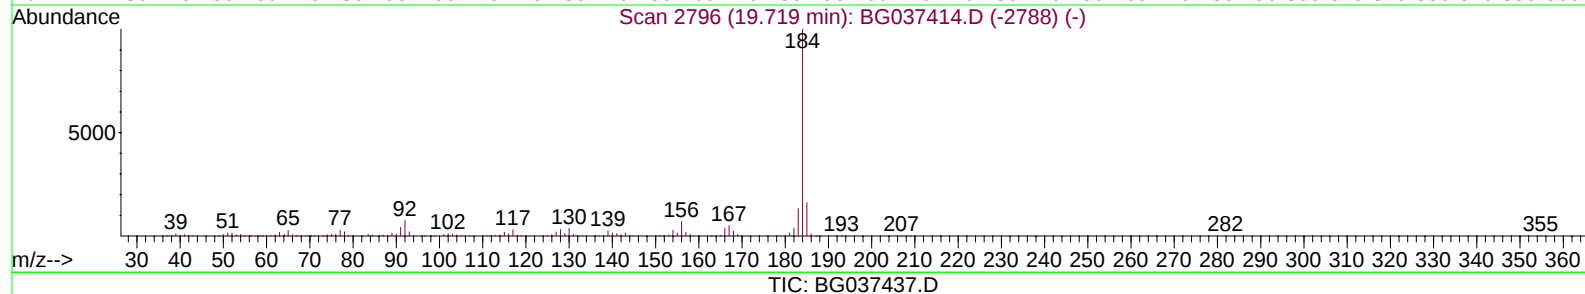
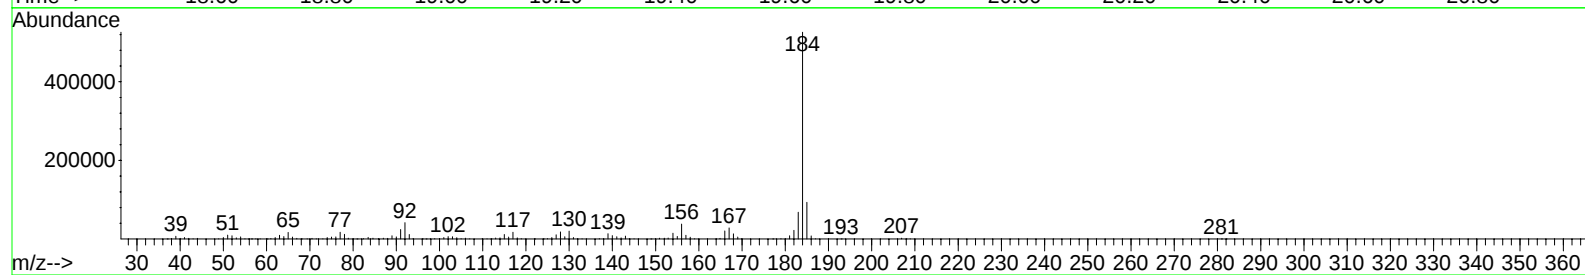


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101818\
Data File : BG037437.D
Acq On : 19 Oct 2018 2:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 11:11:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

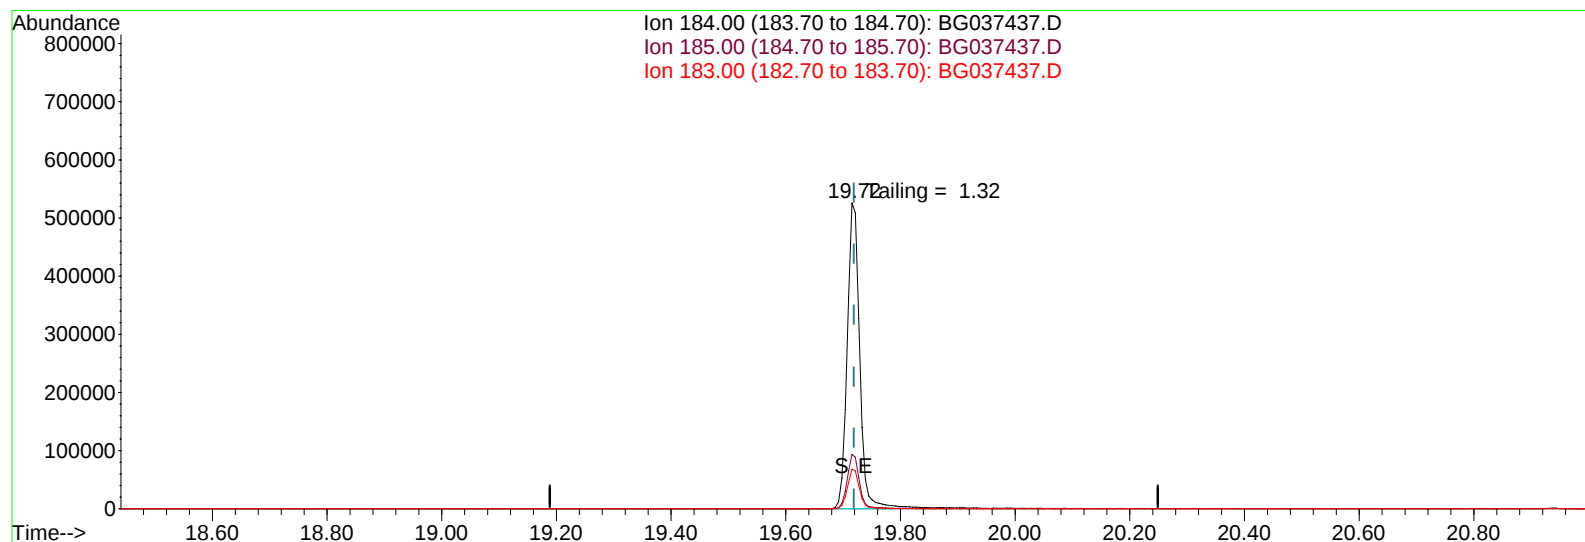

TIC: BG037437.D

(77) Benzidine




19.715min (-0.003) 0.00ng

response 801127

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	17.75
183.00	12.70	12.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101818\
Data File : BG037437.D
Acq On : 19 Oct 2018 2:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 11:11:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

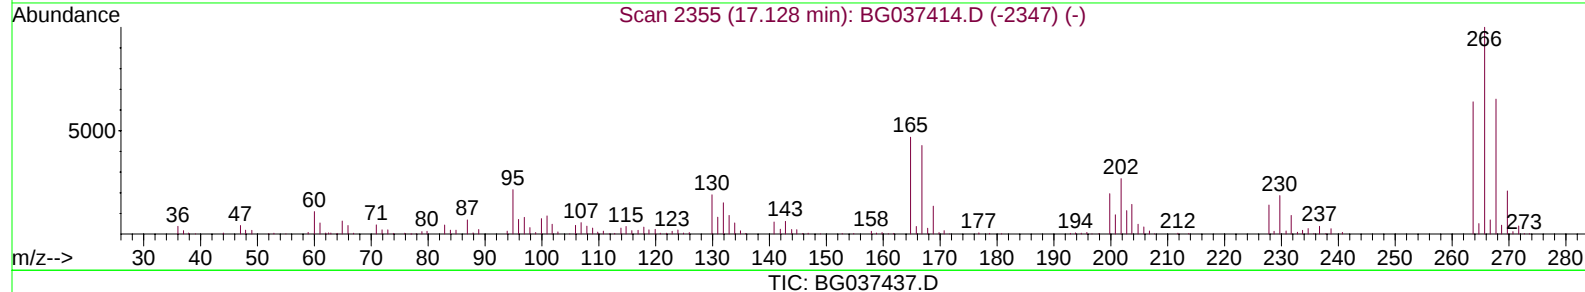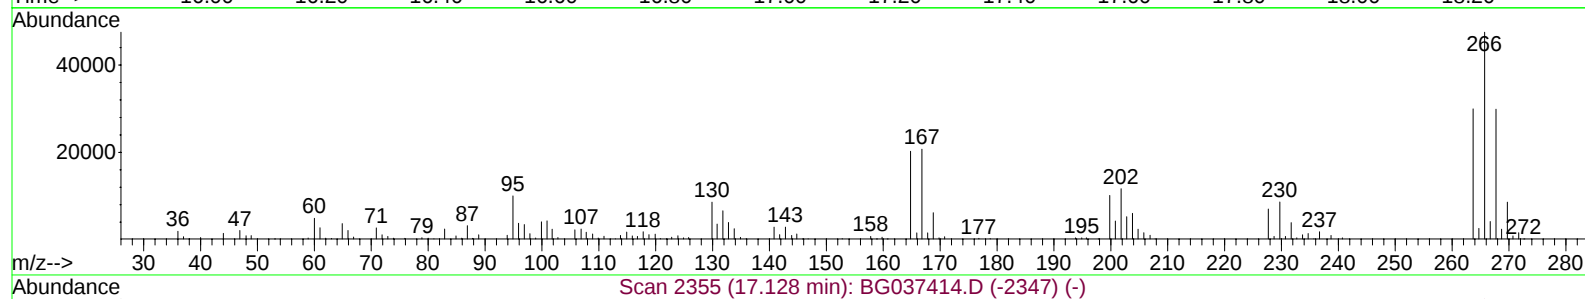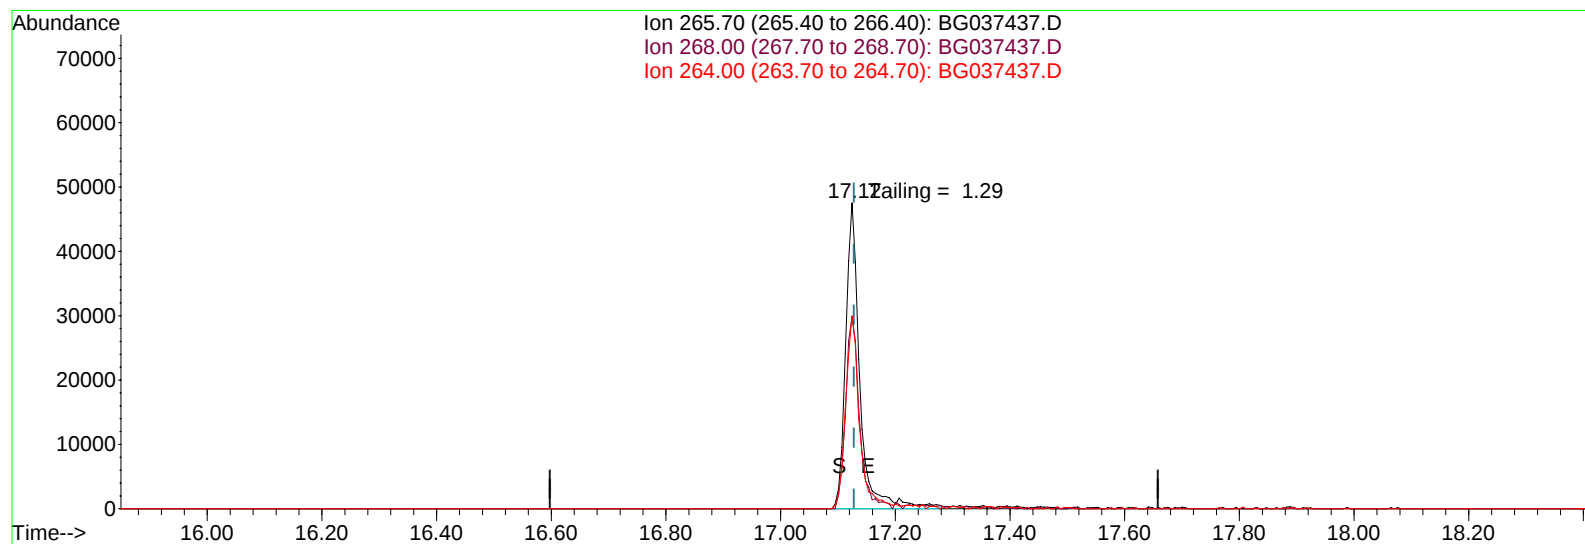

(70) Pentachlorophenol (C)

17.124min (-0.003) 87486.04ng

response 78702

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	67.98
264.00	73.60	68.48
0.00	0.00	0.00