


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG101818\
 Data File : BG037410.D
 Acq On : 18 Oct 2018 8:35
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

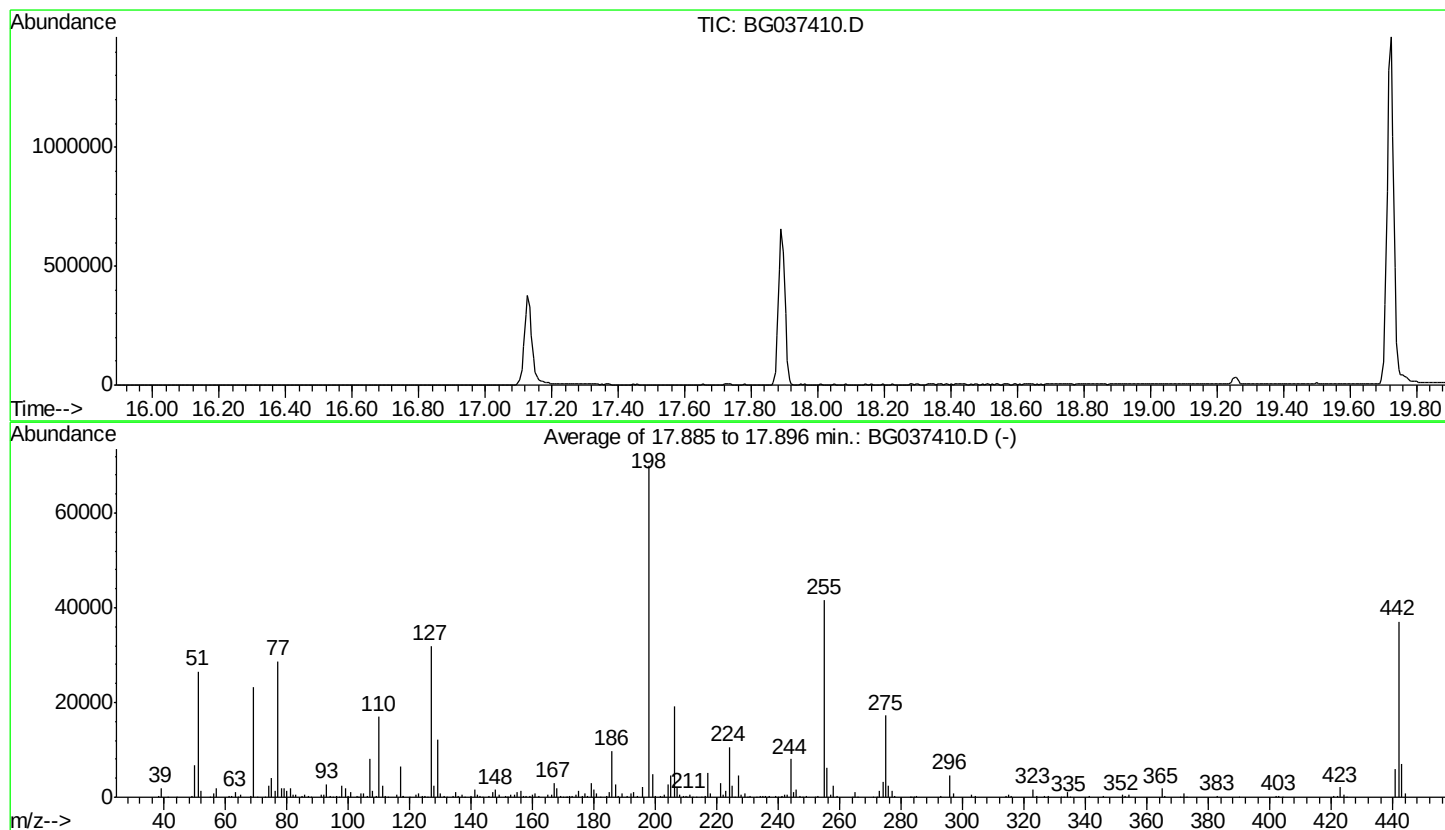

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	26541	PASS
68	69	0.00	2	1.5	354	PASS
69	198	0.00	100	33.3	23301	PASS
70	69	0.00	2	0.3	65	PASS
127	198	10	80	45.6	31904	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	69997	PASS
199	198	5	9	6.8	4750	PASS
275	198	10	60	24.7	17272	PASS
365	198	1	100	2.7	1870	PASS
441	198	0.01	100	8.4	5882	PASS
442	198	50	100	53.0	37082	PASS
443	442	15	24	18.9	7026	PASS