


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101818\
 Data File : BG037419.D
 Acq On : 18 Oct 2018 14:44
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

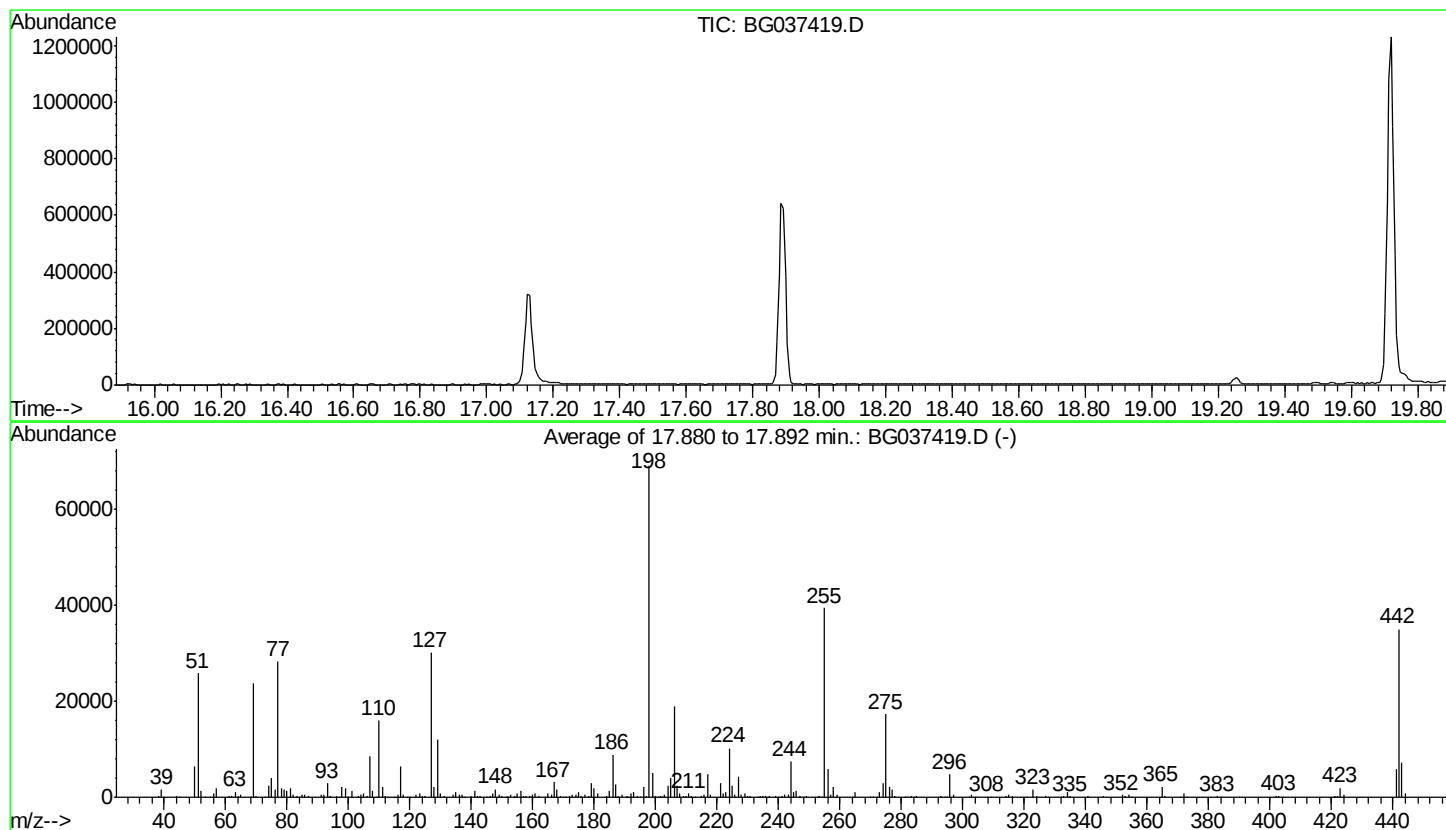

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	25842	PASS
68	69	0.00	2	0.6	142	PASS
69	198	0.00	100	34.3	23656	PASS
70	69	0.00	2	0.6	153	PASS
127	198	10	80	43.6	30112	PASS
197	198	0.00	2	0.3	177	PASS
198	198	100	100	100.0	69042	PASS
199	198	5	9	7.2	4960	PASS
275	198	10	60	25.0	17278	PASS
365	198	1	100	3.2	2209	PASS
441	198	0.01	100	8.6	5940	PASS
442	198	50	100	50.6	34920	PASS
443	442	15	24	20.5	7165	PASS