


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG101818\
Data File : BG037437.D
Acq On : 19 Oct 2018 2:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 18 14:06:42 2018

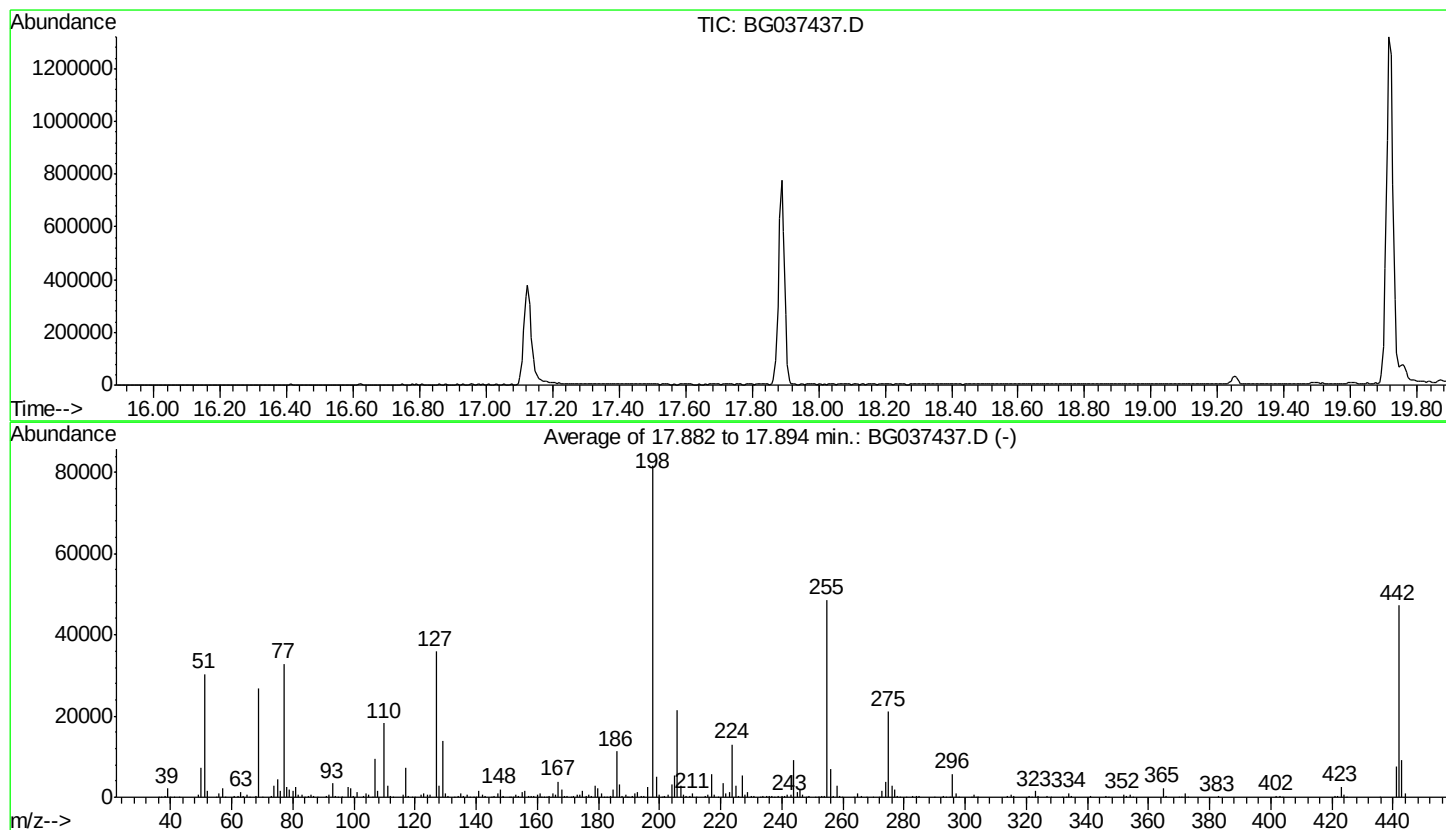

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	30317	PASS
68	69	0.00	2	1.6	439	PASS
69	198	0.00	100	32.8	26781	PASS
70	69	0.00	2	0.2	57	PASS
127	198	10	80	43.9	35848	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	81674	PASS
199	198	5	9	6.4	5210	PASS
275	198	10	60	25.7	20994	PASS
365	198	1	100	2.9	2349	PASS
441	198	0.01	100	9.3	7570	PASS
442	198	50	100	57.8	47224	PASS
443	442	15	24	19.2	9046	PASS