
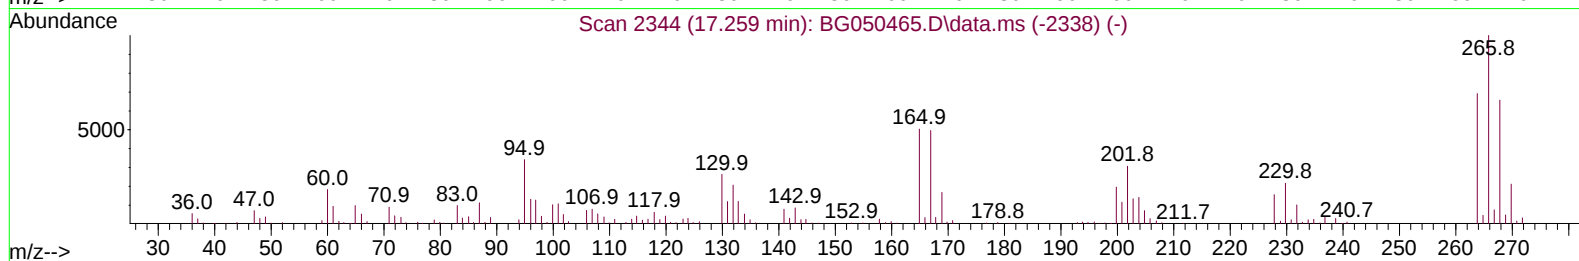
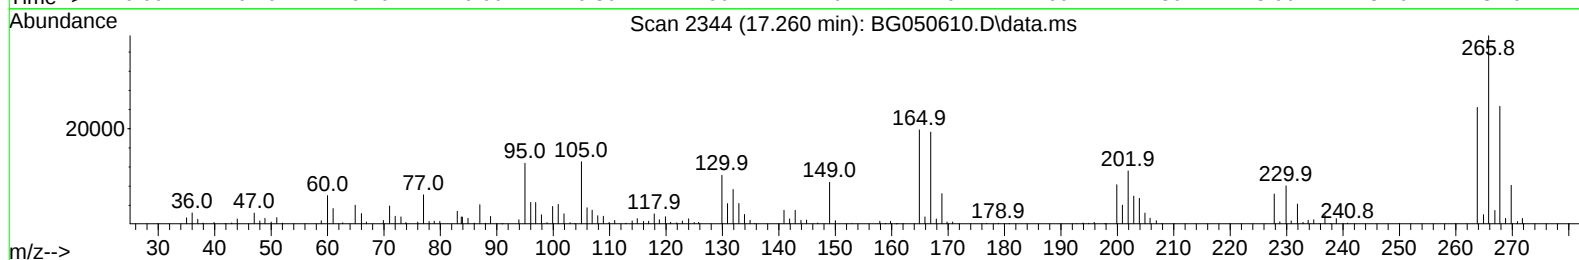


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101821\
Data File : BG050610.D
Acq On : 18 Oct 2021 9:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 10:51:23 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

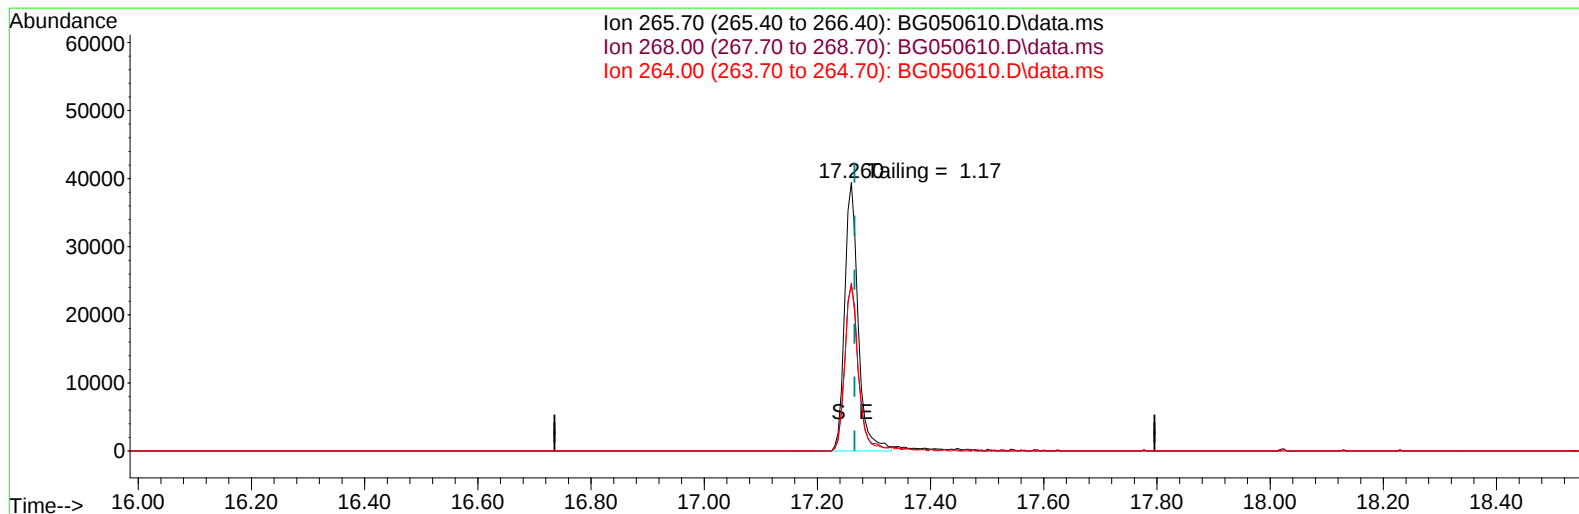

TIC: BG050610.D\data.ms

(70) Pentachlorophenol (C)




17.260min (-0.005) 22366.49 ng

response 67706

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.57
264.00	61.30	61.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101821\
Data File : BG050610.D
Acq On : 18 Oct 2021 9:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 10:51:23 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

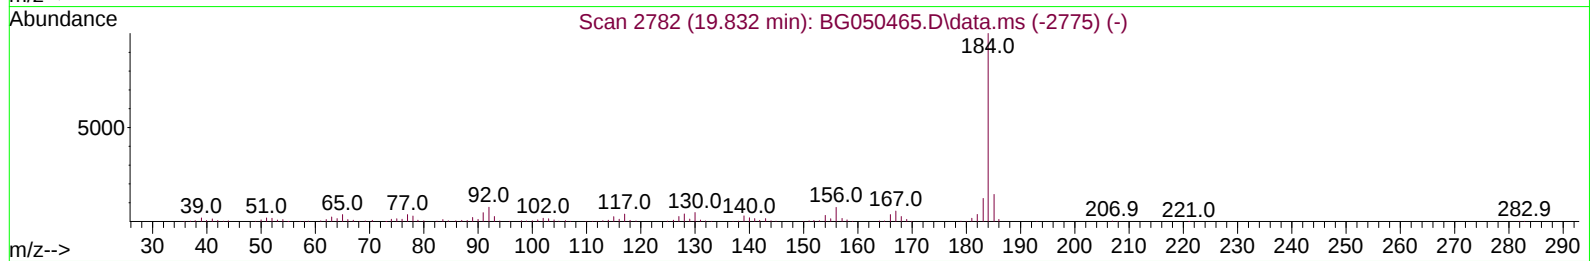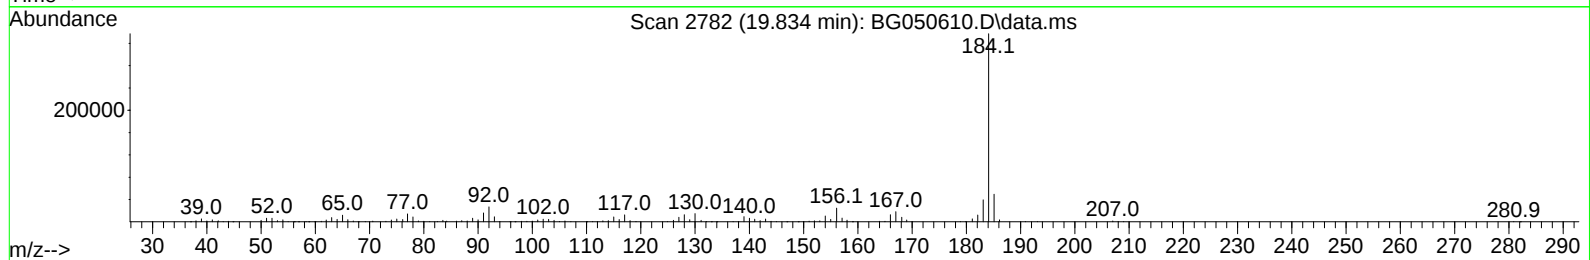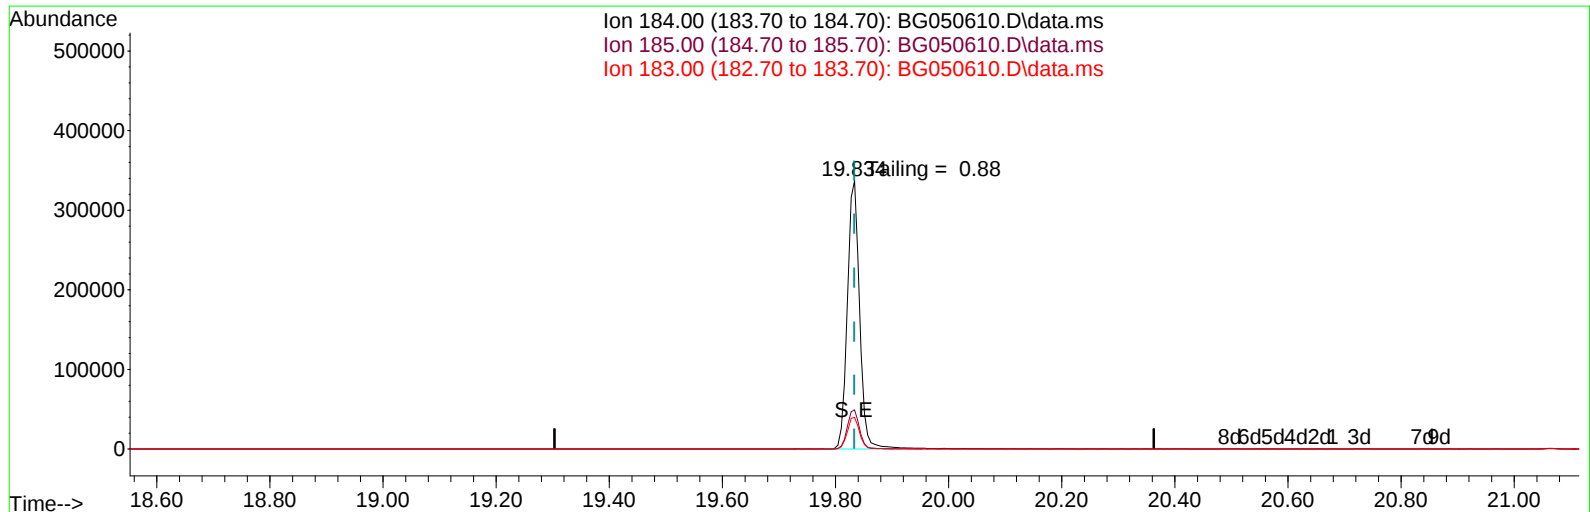

TIC: BG050610.D\data.ms

(77) Benzidine

19.834min (+ 0.001) 296751.81 ng m

response 509758

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.64
183.00	11.70	11.74
0.00	0.00	0.00