


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101821\
 Data File : BG050610.D
 Acq On : 18 Oct 2021 9:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 14 10:56:22 2021

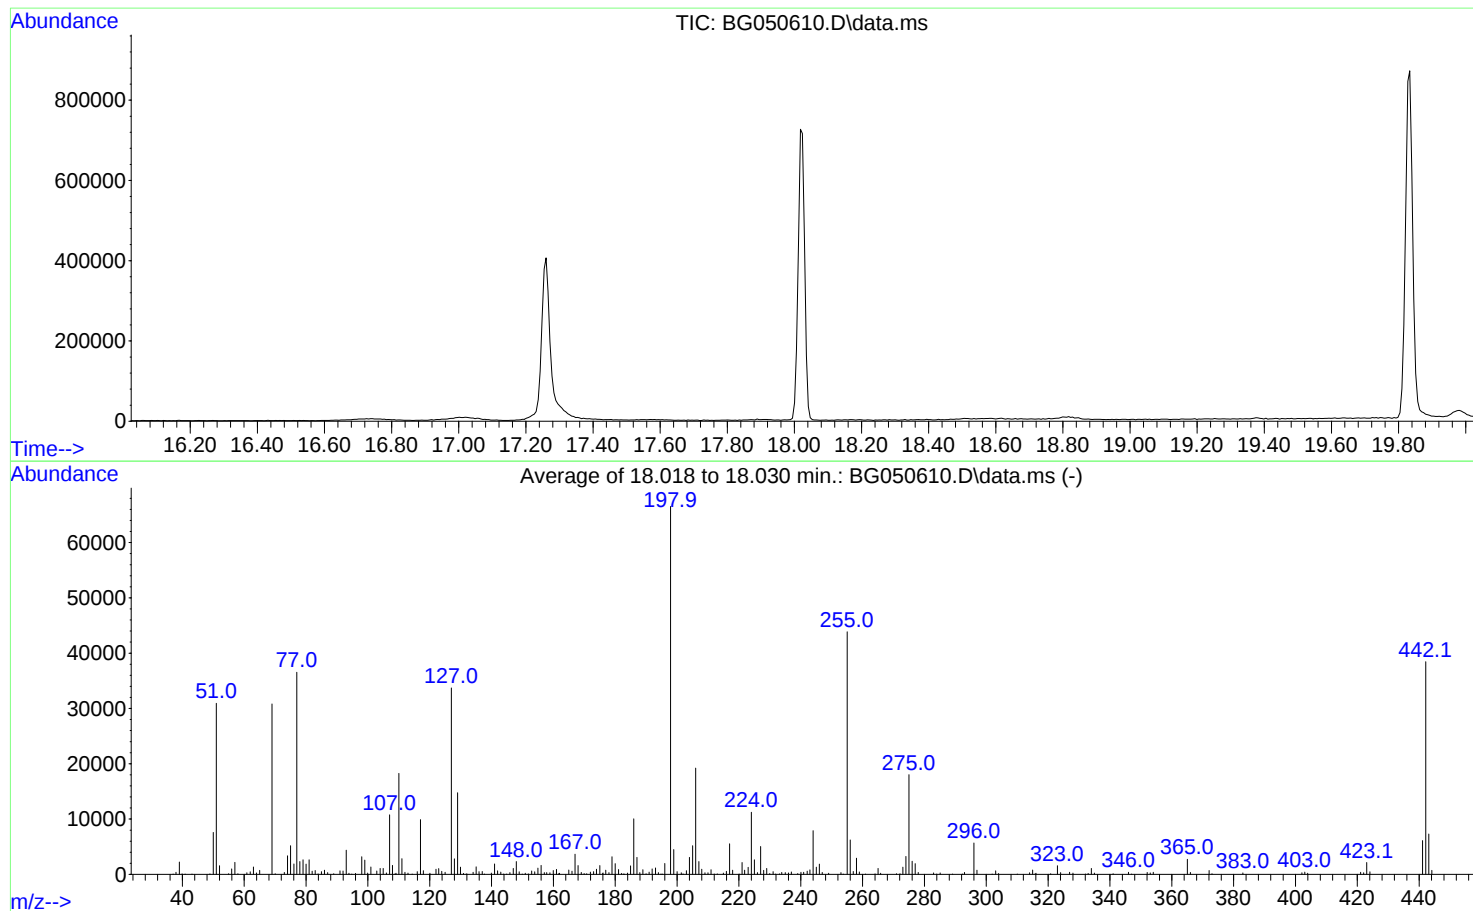




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.5	30936	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.3	30806	PASS
70	69	0.00	2	0.4	127	PASS
127	198	10	80	50.7	33717	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	66520	PASS
199	198	5	9	6.7	4473	PASS
275	198	10	60	27.1	18015	PASS
365	198	1	100	4.1	2724	PASS
441	198	0.01	100	9.2	6112	PASS
442	442	50	100	100.0	38459	PASS
443	442	15	24	18.9	7286	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101821\
Data File : BG050610.D
Acq On : 18 Oct 2021 9:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 18 10:51:23 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

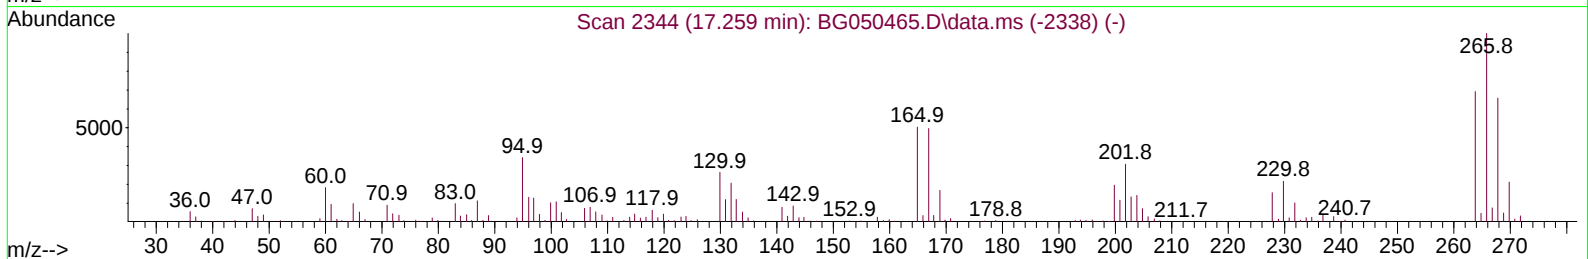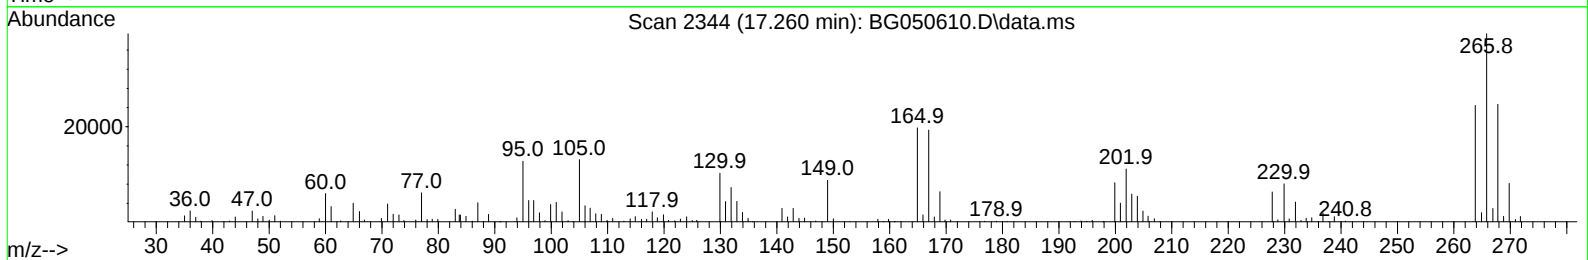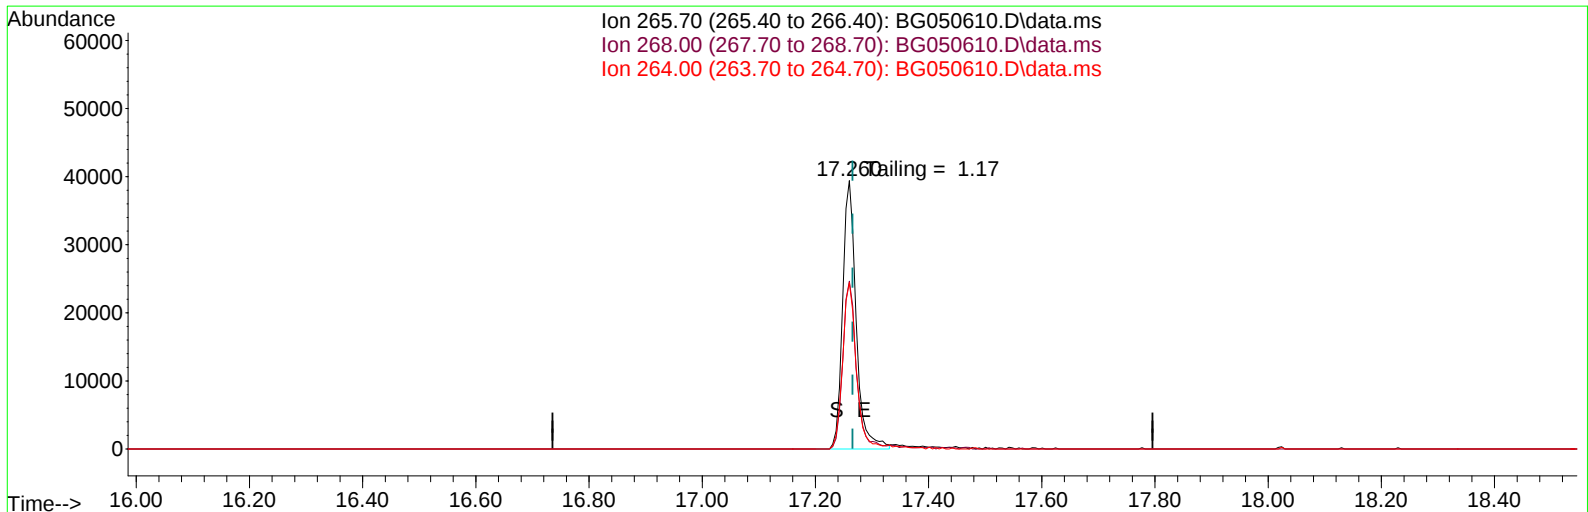

TIC: BG050610.D\data.ms

(70) Pentachlorophenol (C)

17.260min (-0.005) 22366.49 ng




response 67706

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.57
264.00	61.30	61.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101821\
Data File : BG050610.D
Acq On : 18 Oct 2021 9:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 18 10:51:23 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

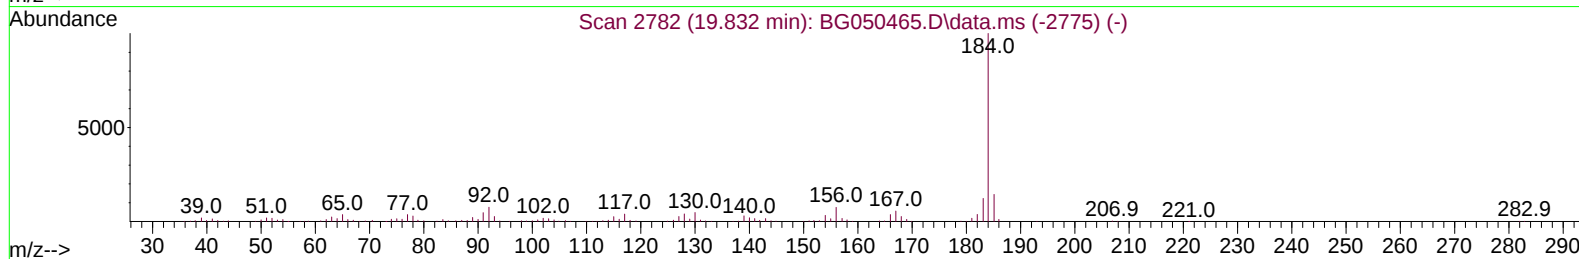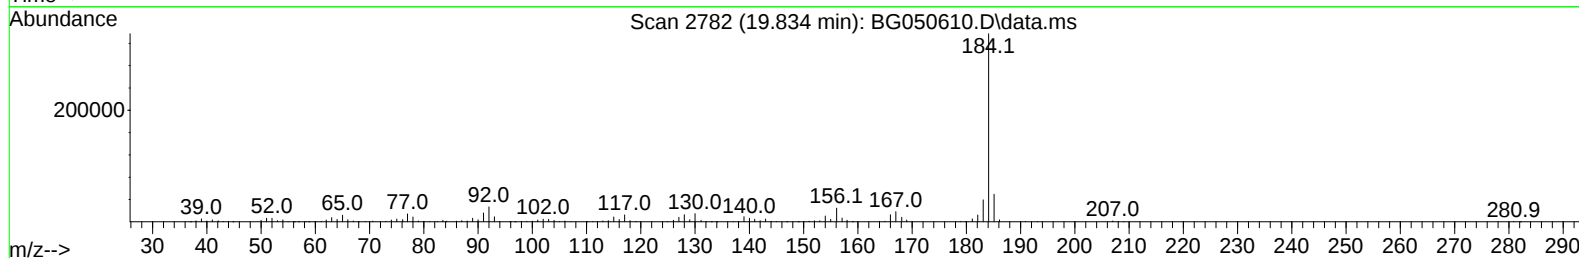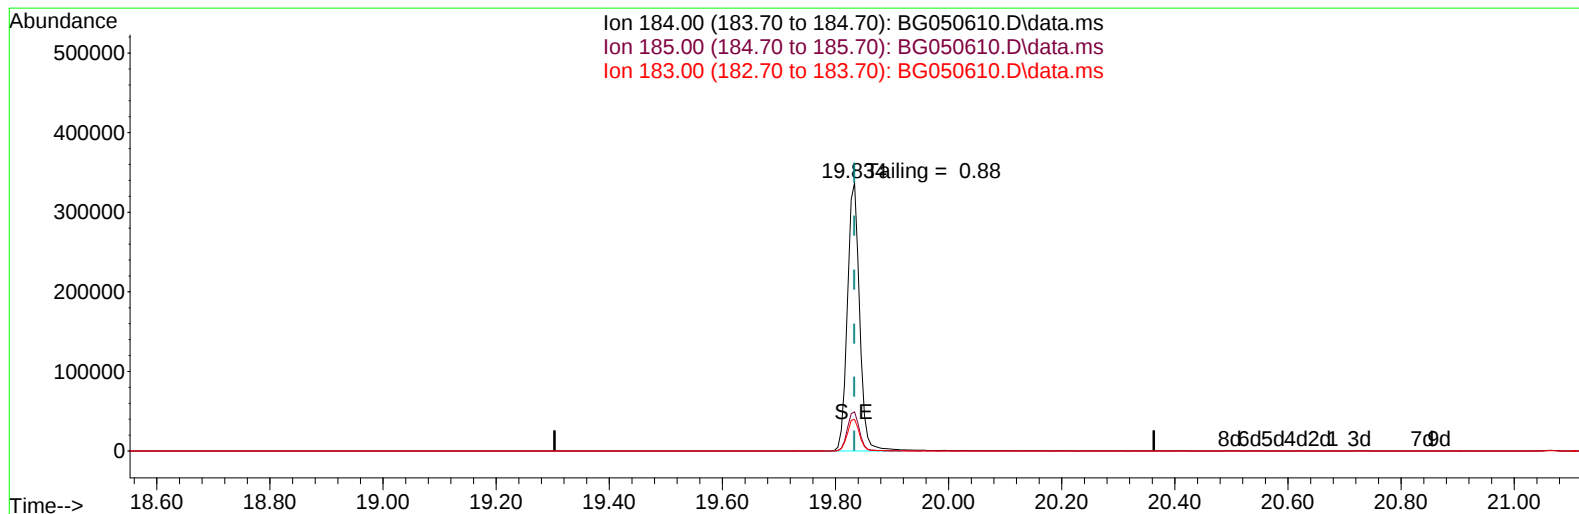

TIC: BG050610.D\data.ms

(77) Benzidine

19.834min (+ 0.001) 296751.81 ng m

response 509758

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.64
183.00	11.70	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/18/2021	BNA_G	BG050610.D
Compound Name	Response	Retention Time
DDT	221653	21.06
DDD	4551	20.61
DDE	1096	20.11
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5647	227300	2.48

Instrument :
BNA_G
ClientSampleId :
DFTPP