
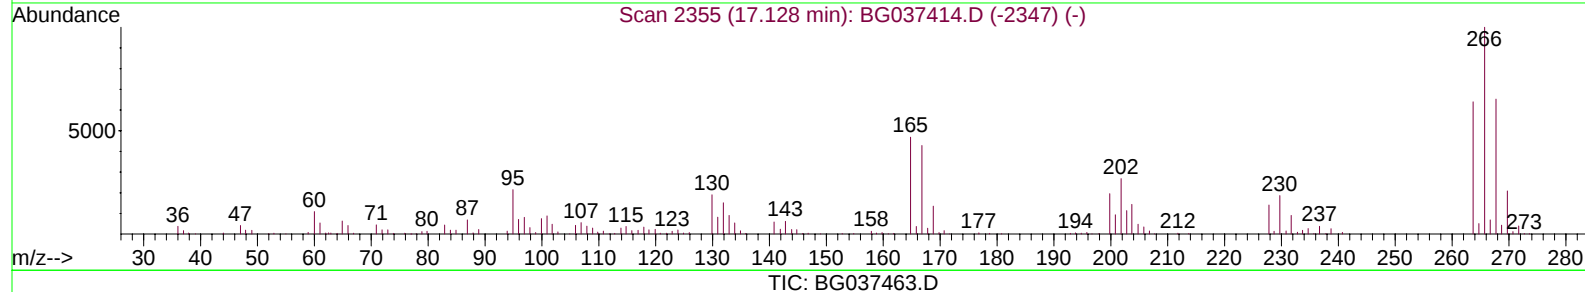
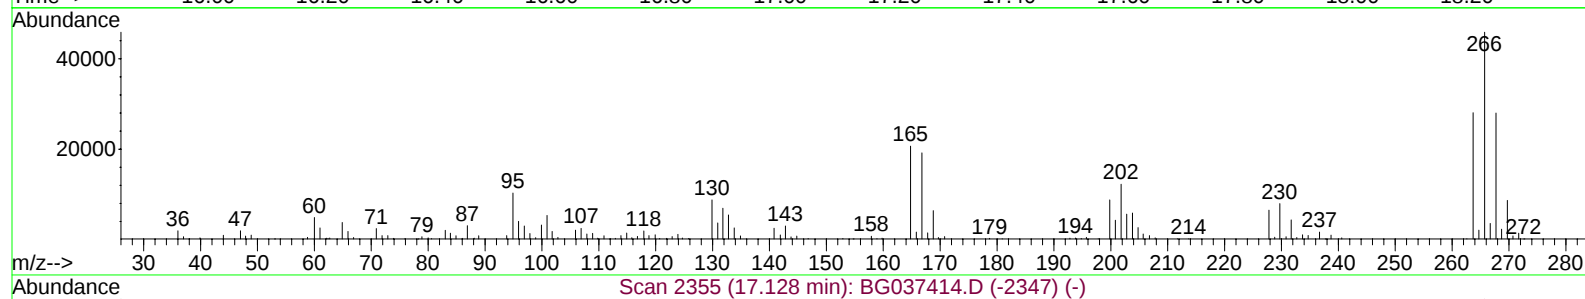


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101918\
Data File : BG037463.D
Acq On : 19 Oct 2018 23:07
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 09:37:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

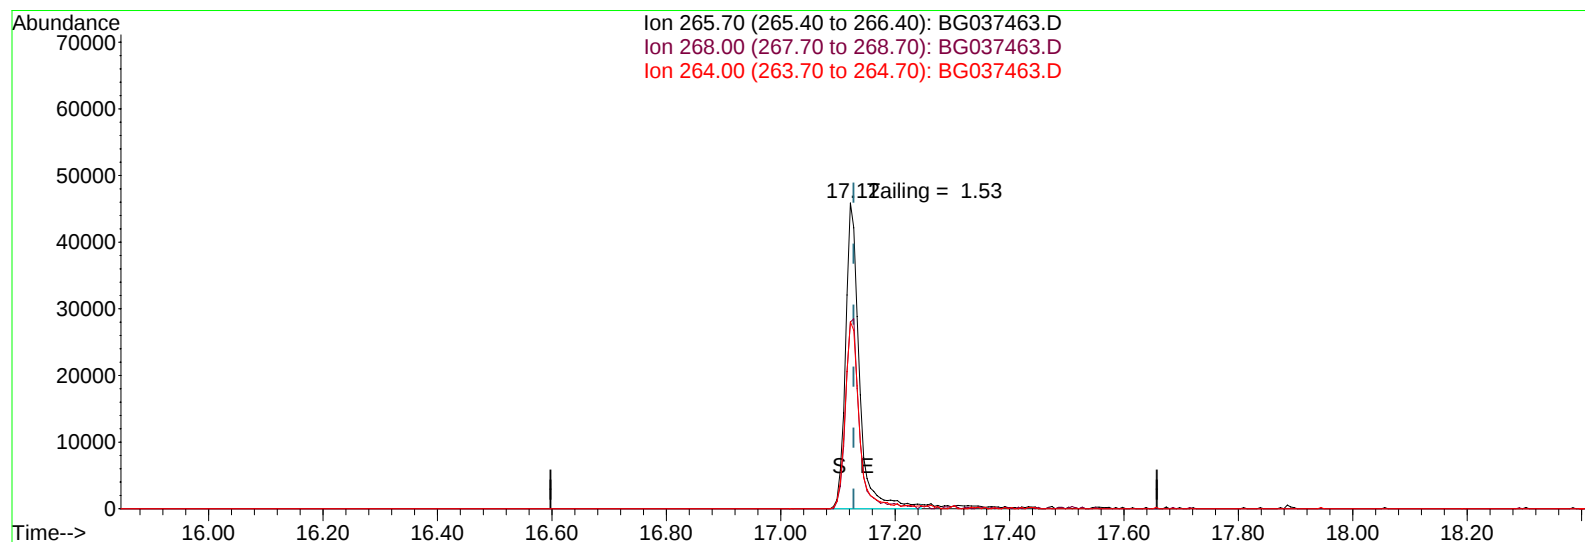

(70) Pentachlorophenol (C)




17.122min (-0.006) 166203.33ng

response 77292

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	66.14
264.00	73.60	65.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101918\
Data File : BG037463.D
Acq On : 19 Oct 2018 23:07
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 09:37:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

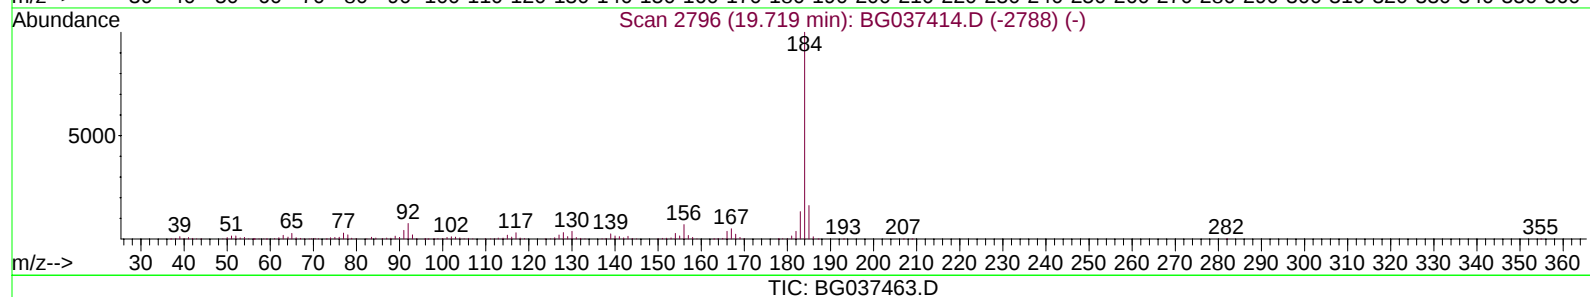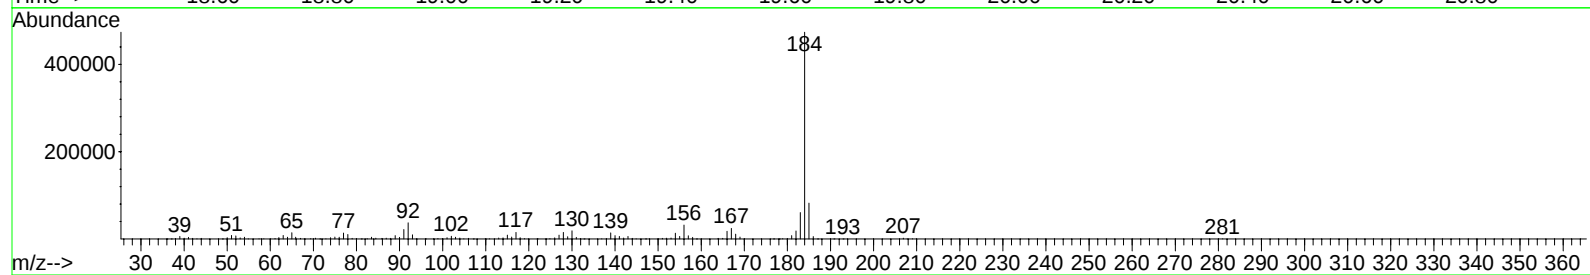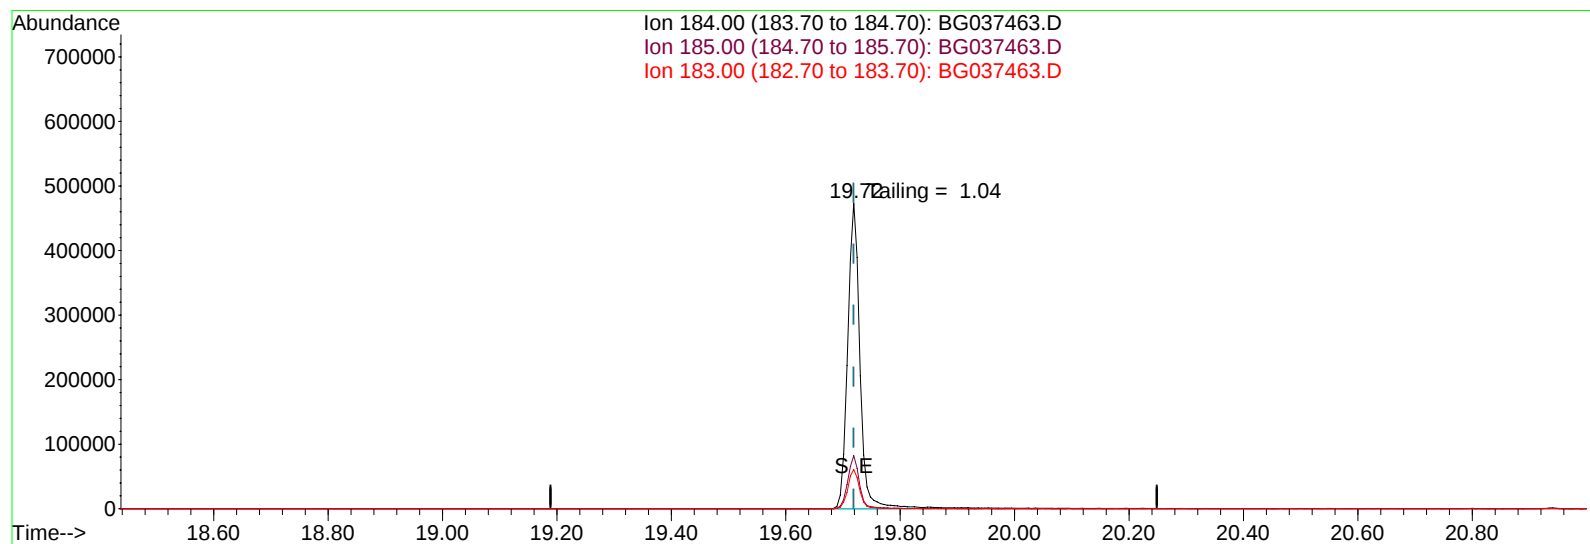

(77) Benzidine

19.719min (-0.000) 0.00ng

response 706210

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	17.36
183.00	12.70	12.81
0.00	0.00	0.00