


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG101918\  
 Data File : BG037445.D  
 Acq On : 19 Oct 2018 9:09  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG101818.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Oct 18 14:06:42 2018

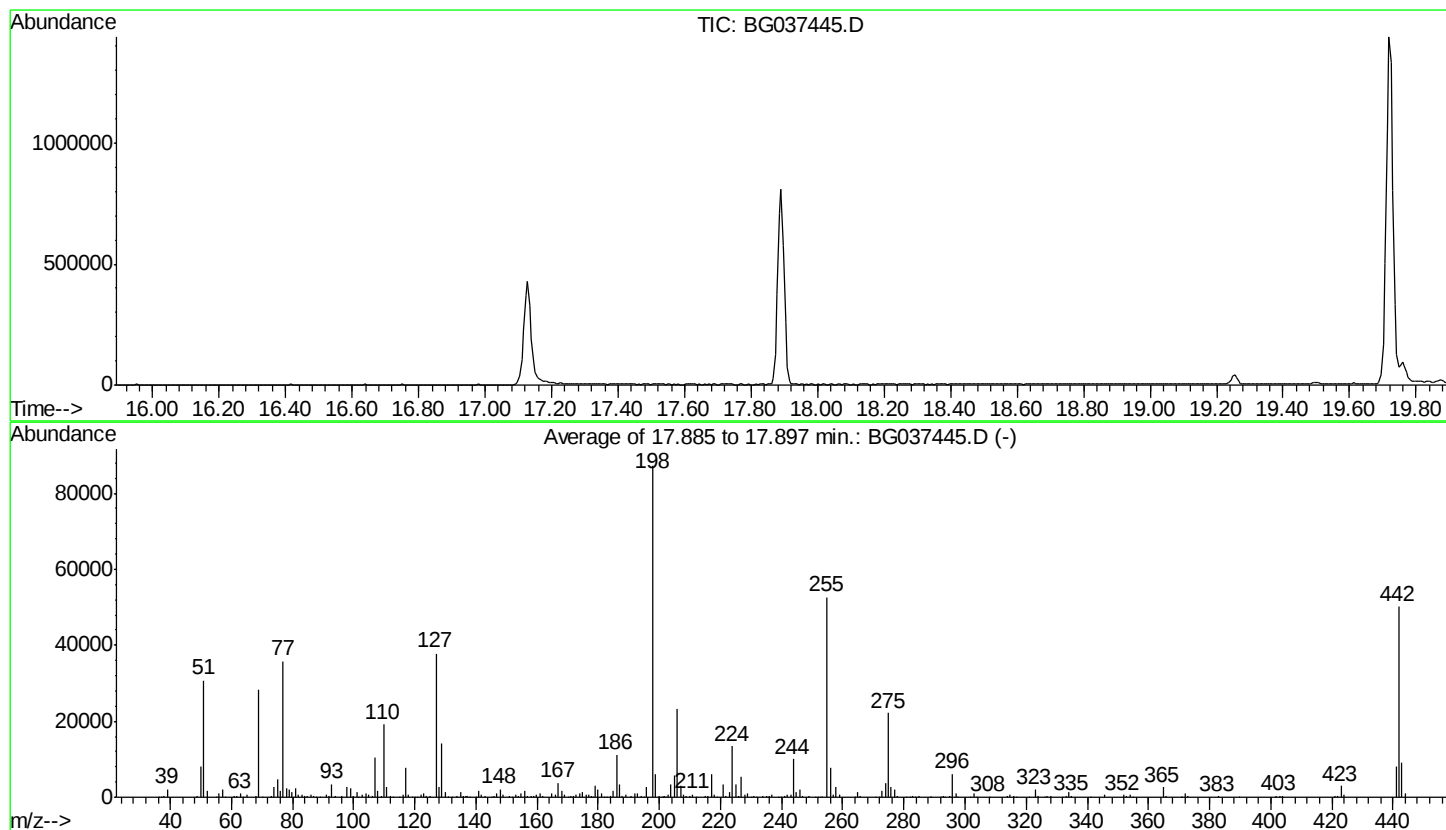

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 35.2      | 30685   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.2       | 334     | PASS             |
| 69          | 198          | 0.00         | 100          | 32.5      | 28381   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 144     | PASS             |
| 127         | 198          | 10           | 80           | 43.4      | 37845   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 87269   | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 5910    | PASS             |
| 275         | 198          | 10           | 60           | 25.5      | 22229   | PASS             |
| 365         | 198          | 1            | 100          | 2.9       | 2561    | PASS             |
| 441         | 198          | 0.01         | 100          | 9.3       | 8086    | PASS             |
| 442         | 198          | 50           | 100          | 57.4      | 50090   | PASS             |
| 443         | 442          | 15           | 24           | 18.2      | 9136    | PASS             |