


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG101918\
 Data File : BG037463.D
 Acq On : 19 Oct 2018 23:07
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

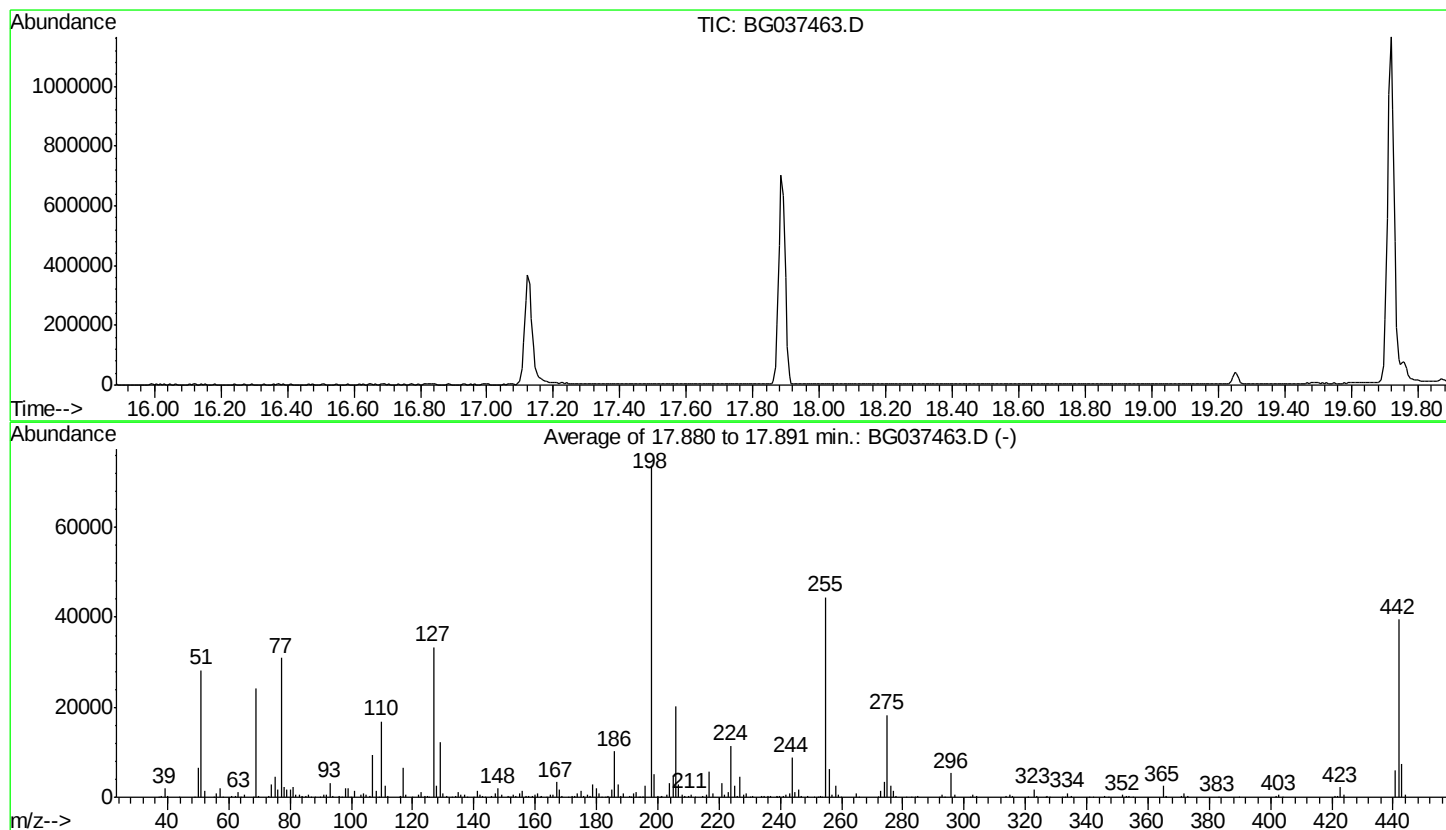

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	28216	PASS
68	69	0.00	2	0.4	107	PASS
69	198	0.00	100	32.9	24234	PASS
70	69	0.00	2	0.8	201	PASS
127	198	10	80	45.2	33296	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	73709	PASS
199	198	5	9	6.8	5037	PASS
275	198	10	60	24.8	18308	PASS
365	198	1	100	3.3	2444	PASS
441	198	0.01	100	8.1	5963	PASS
442	198	50	100	53.6	39514	PASS
443	442	15	24	18.8	7419	PASS