
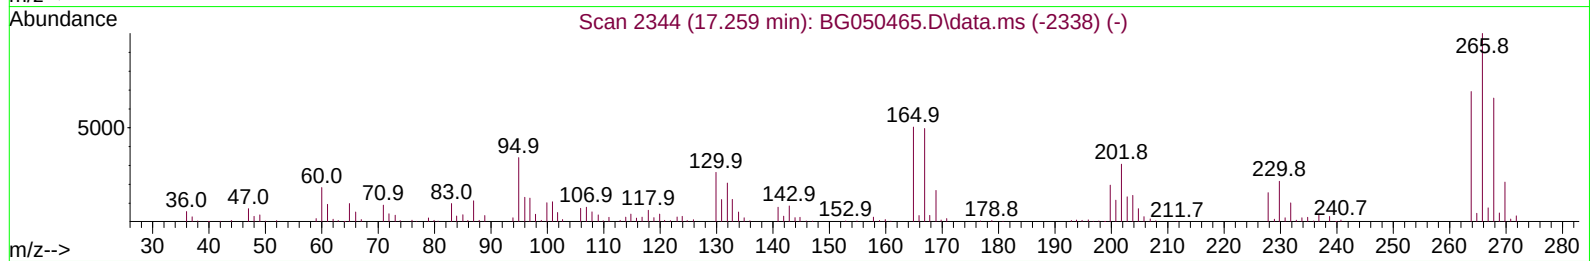
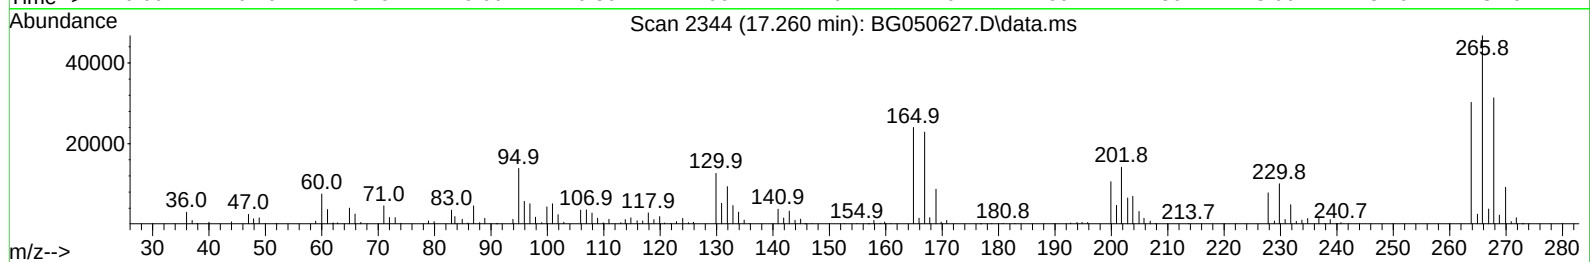


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101921\
Data File : BG050627.D
Acq On : 19 Oct 2021 9:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 19 09:55:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

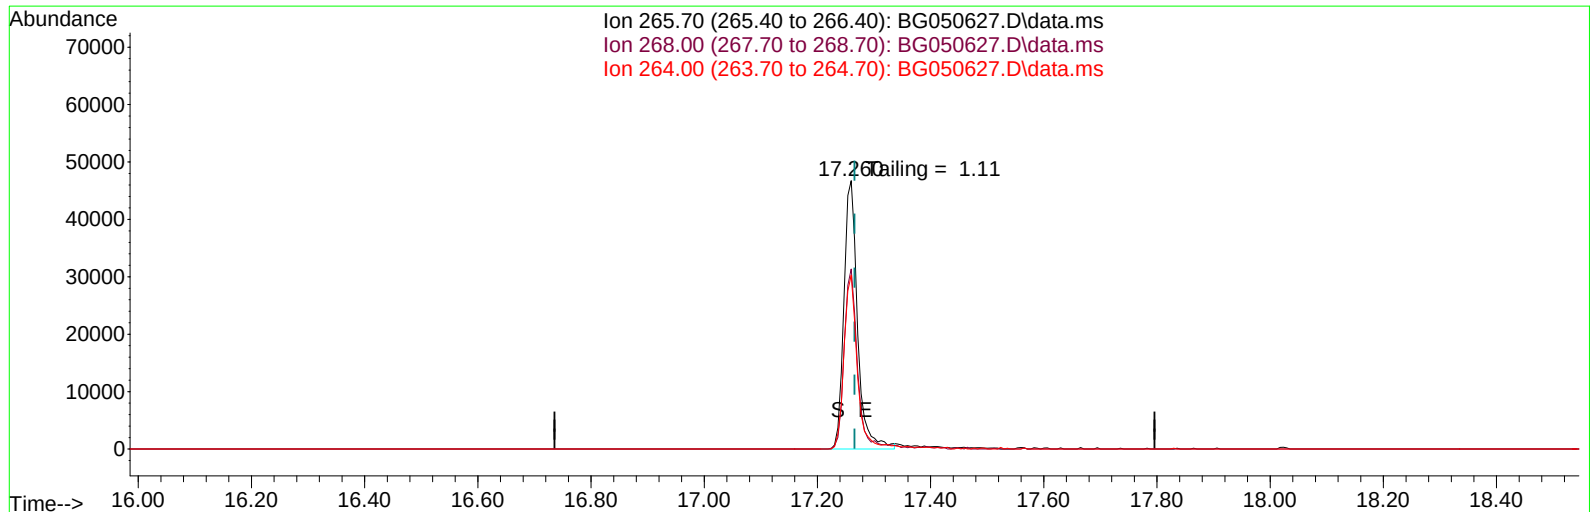

TIC: BG050627.D\data.ms

(70) Pentachlorophenol (C)




17.260min (-0.006) 17302.88 ng

response 77741

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	67.08
264.00	61.30	64.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101921\
Data File : BG050627.D
Acq On : 19 Oct 2021 9:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 19 09:55:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

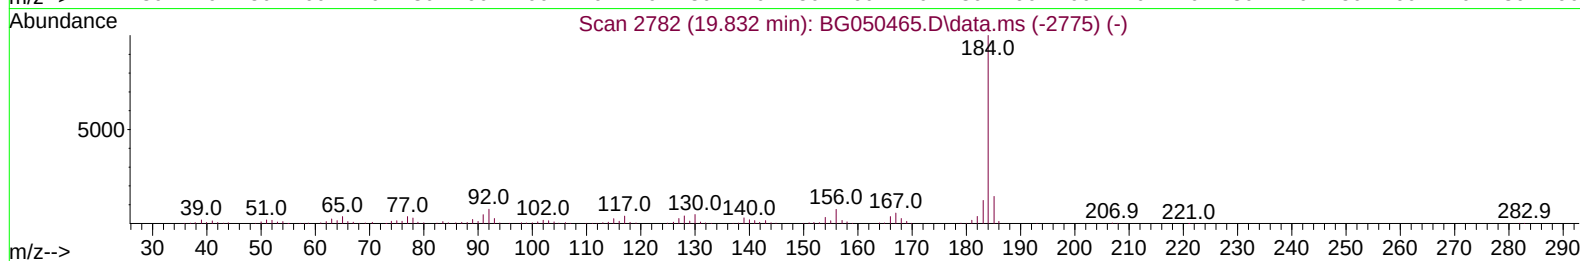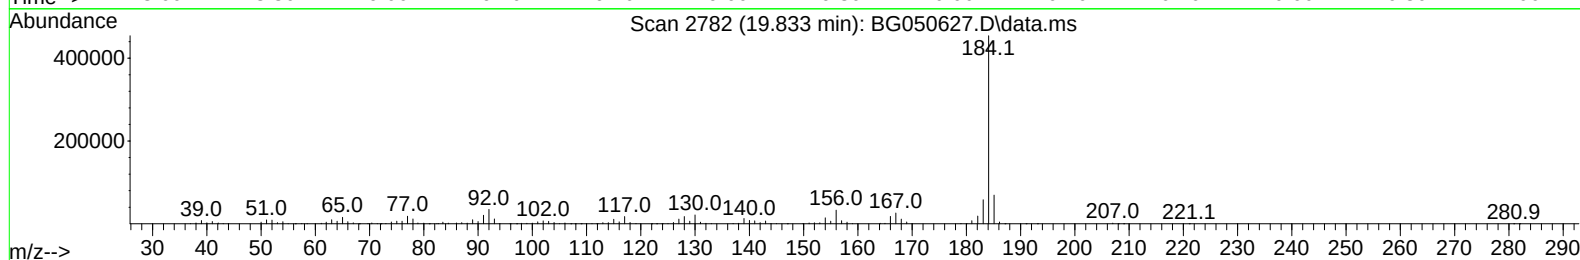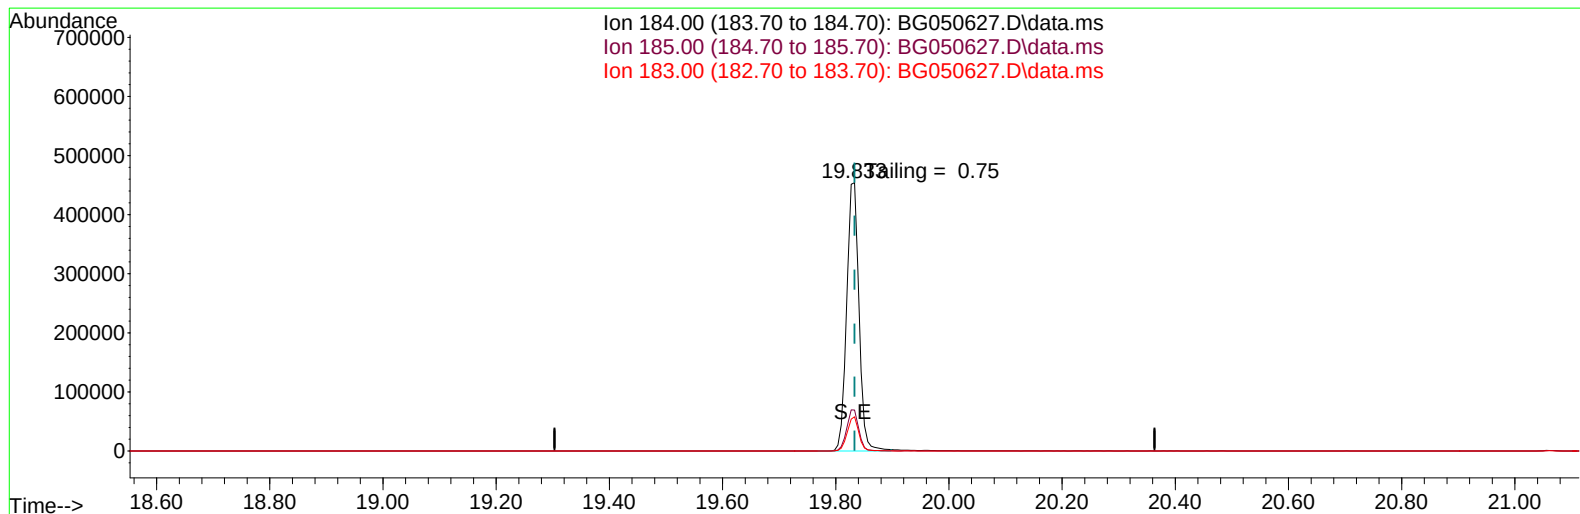

TIC: BG050627.D\data.ms

(77) Benzidine

19.833min (+ 0.000) 0.00 ng

response 691199

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.29
183.00	11.70	12.77
0.00	0.00	0.00