


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101921\
 Data File : BG050627.D
 Acq On : 19 Oct 2021 9:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 14 10:56:22 2021

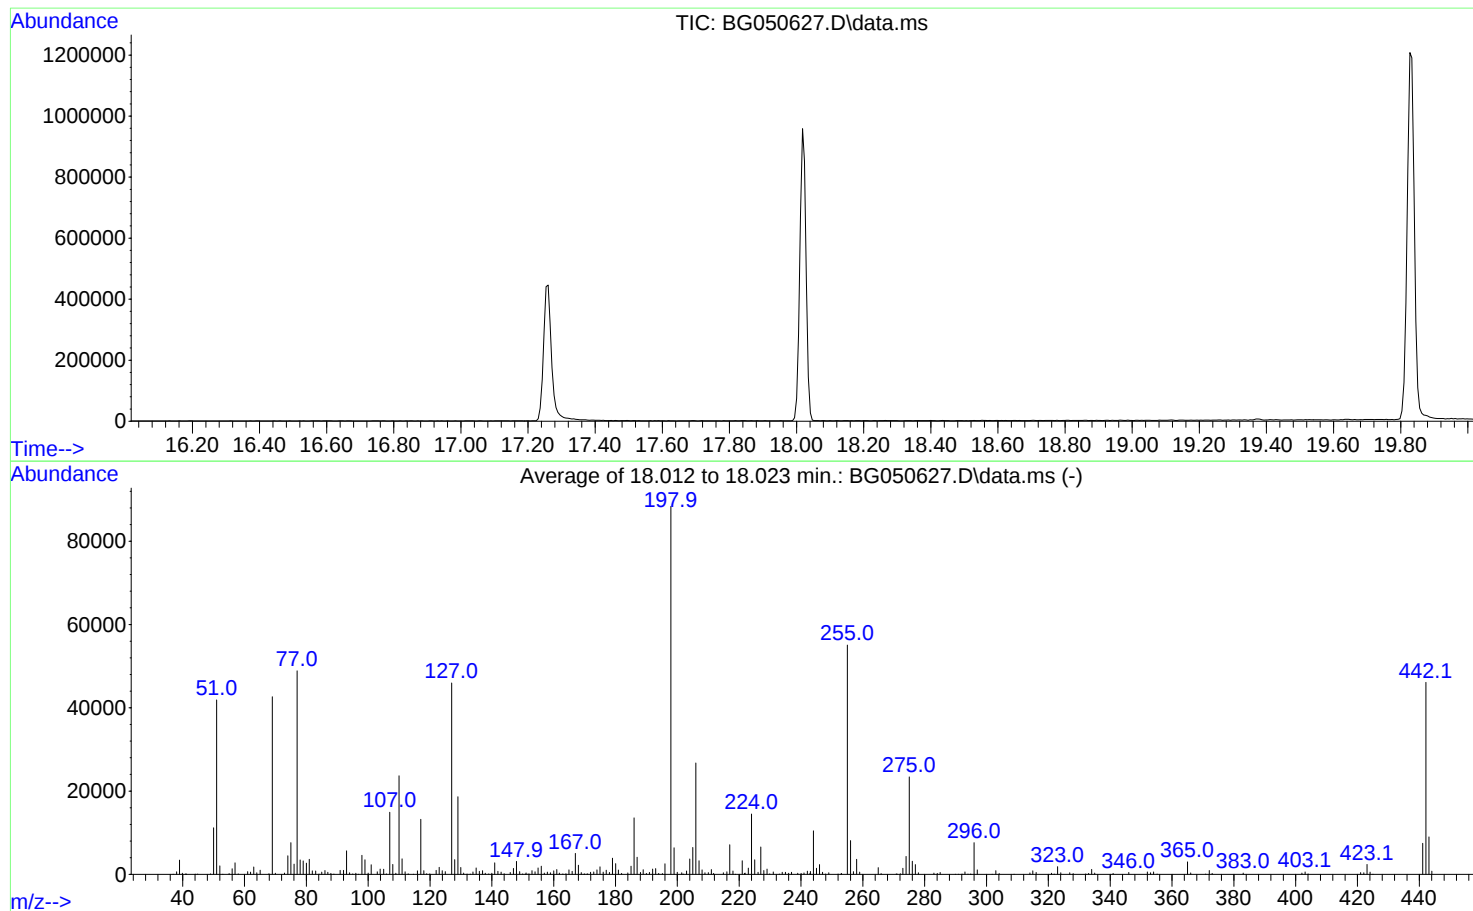




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.4	41896	PASS
68	69	0.00	2	0.3	145	PASS
69	198	0.00	100	48.3	42643	PASS
70	69	0.00	2	0.6	256	PASS
127	198	10	80	52.0	45949	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	88344	PASS
199	198	5	9	7.2	6386	PASS
275	198	10	60	26.5	23384	PASS
365	198	1	100	3.4	2986	PASS
441	198	0.01	100	8.4	7464	PASS
442	442	50	100	100.0	46101	PASS
443	442	15	24	19.5	8980	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101921\
Data File : BG050627.D
Acq On : 19 Oct 2021 9:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 19 09:55:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

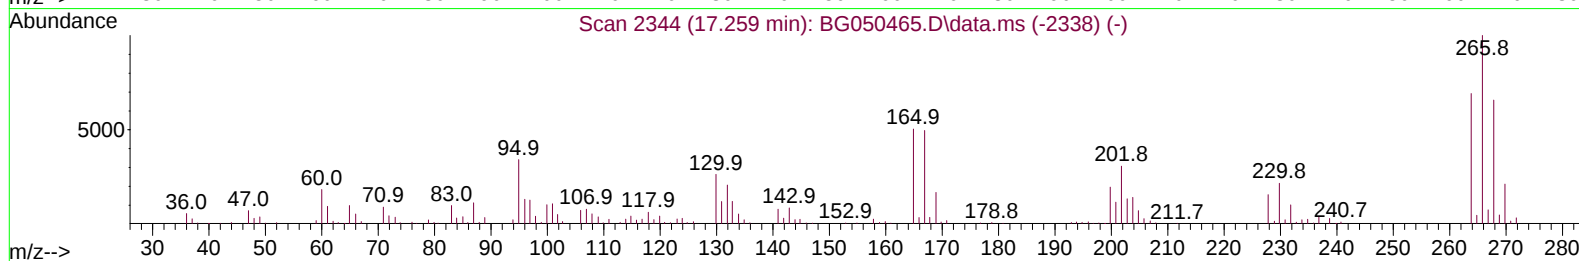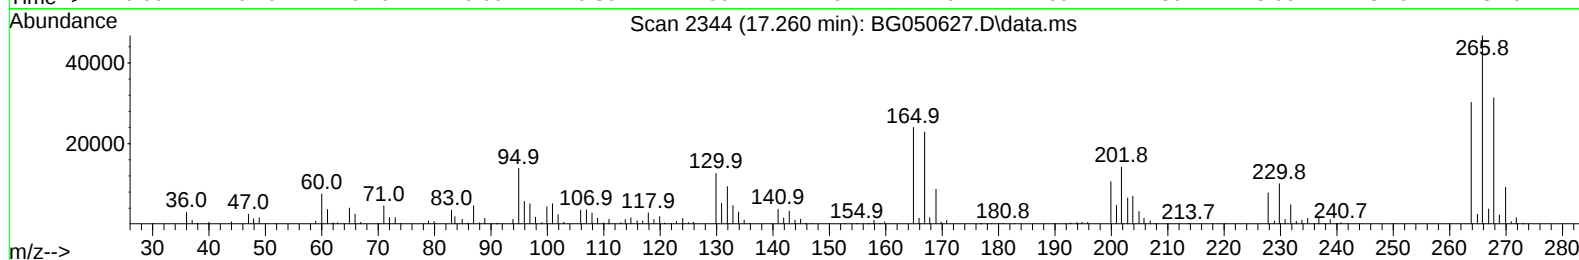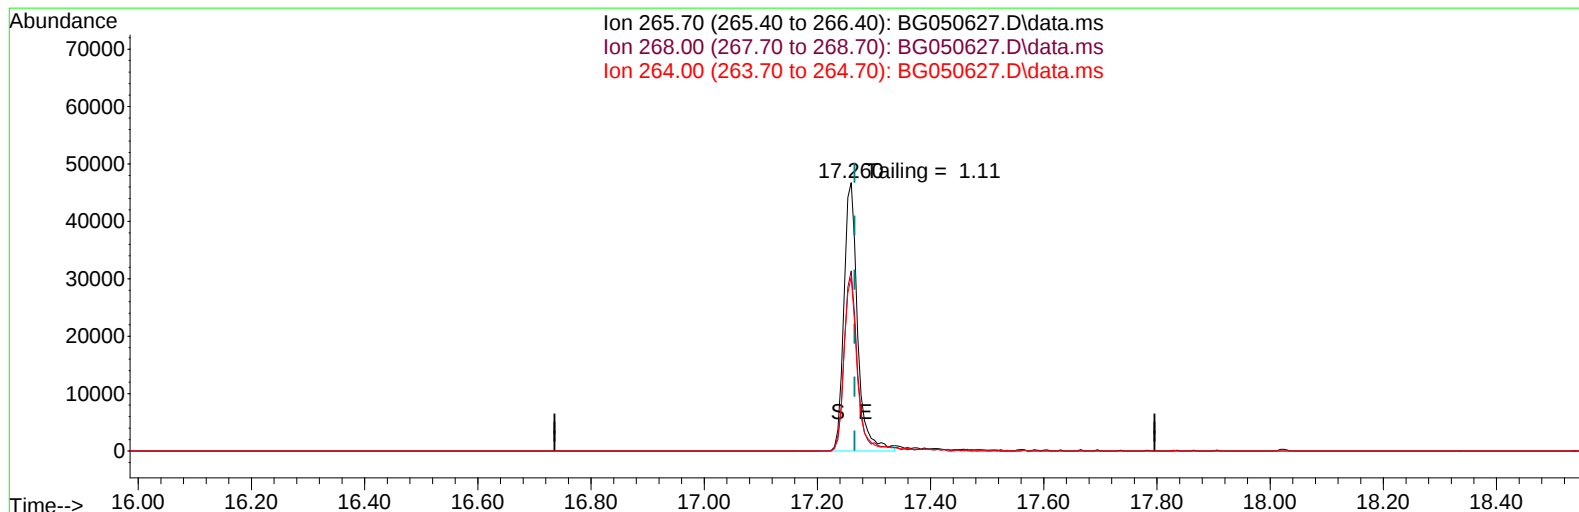

TIC: BG050627.D\data.ms

(70) Pentachlorophenol (C)

17.260min (-0.006) 17302.88 ng




response 77741

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	67.08
264.00	61.30	64.75
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101921\  
Data File : BG050627.D  
Acq On    : 19 Oct 2021    9:11  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 19 09:55:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

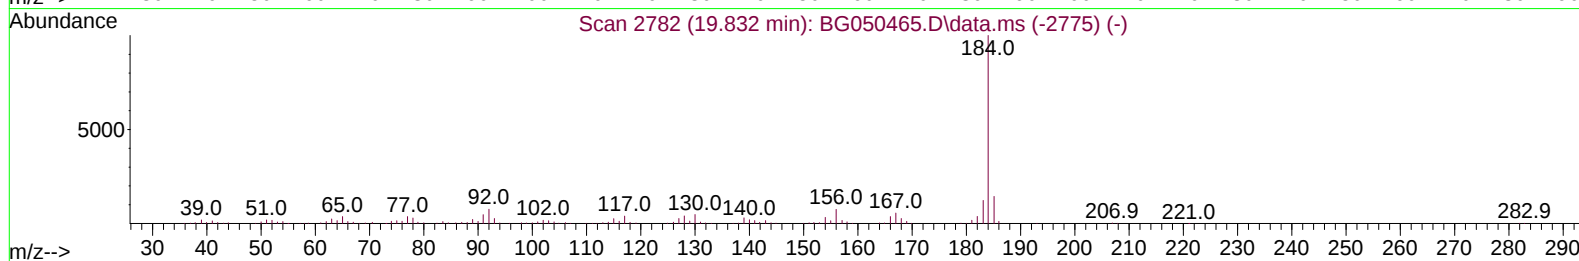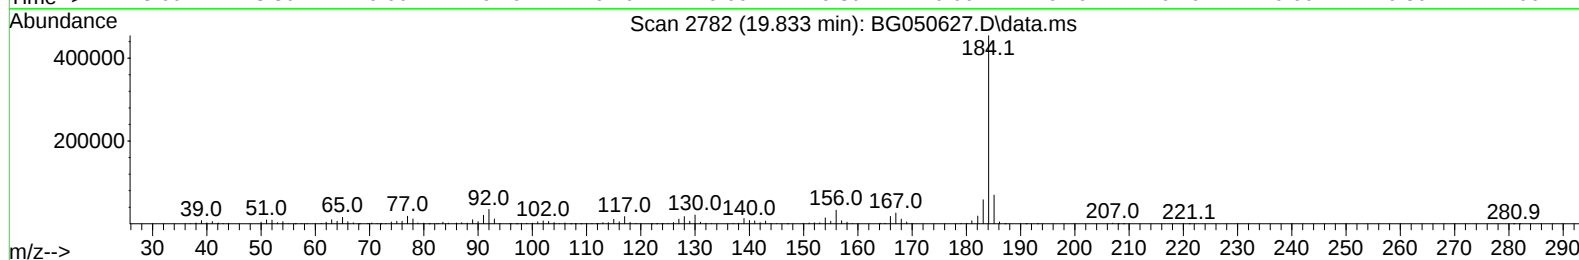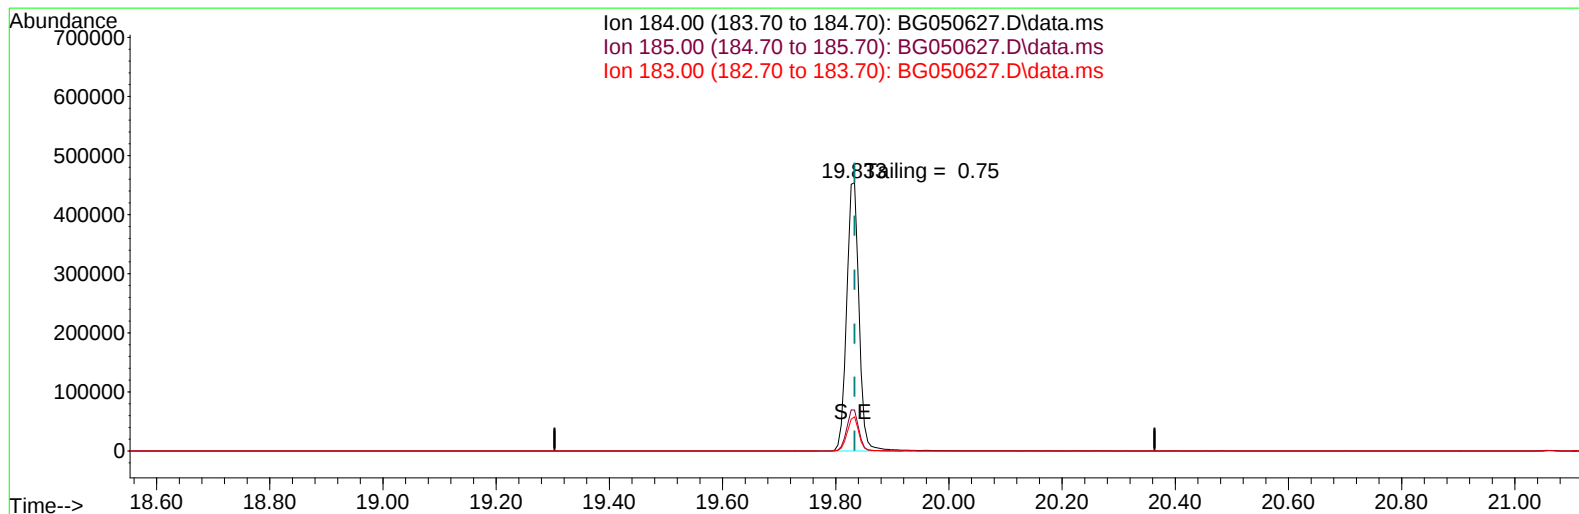

TIC: BG050627.D\data.ms

(77) Benzidine

19.833min (+ 0.000) 0.00 ng

response **691199**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.29
183.00	11.70	12.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/19/2021	BNA_G	BG050627.D
Compound Name	Response	Retention Time
DDT	308629	21.06
DDD	7153	20.6
DDE	984	20.1
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8137	316766	2.57

Instrument :
BNA_G
ClientSampleId :
DFTPP