
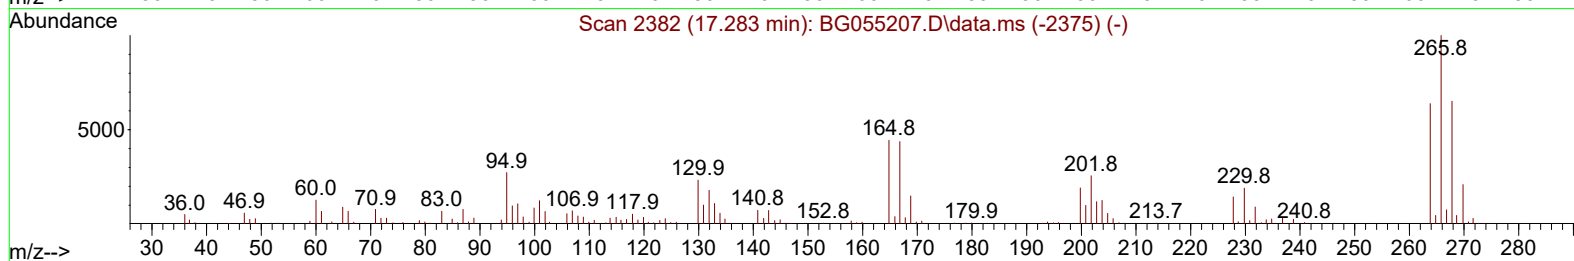
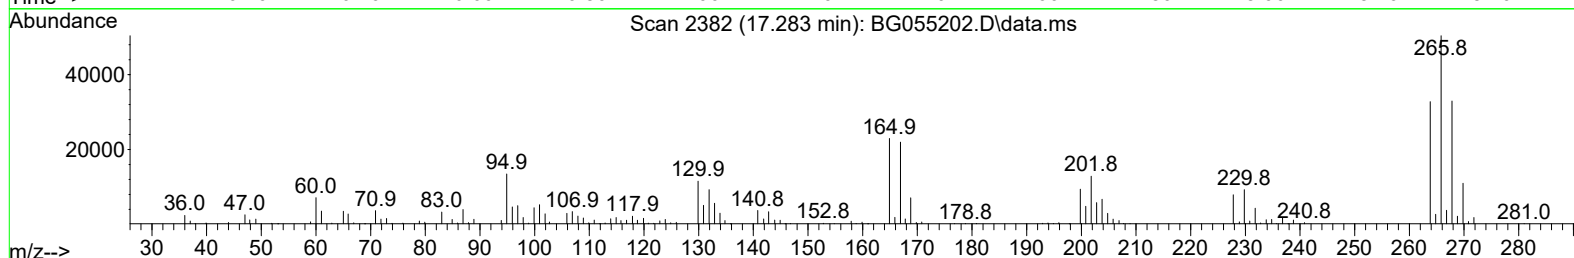


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101922\
Data File : BG055202.D
Acq On : 19 Oct 2022 10:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 20 10:07:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 20 09:21:42 2022
Response via : Initial Calibration

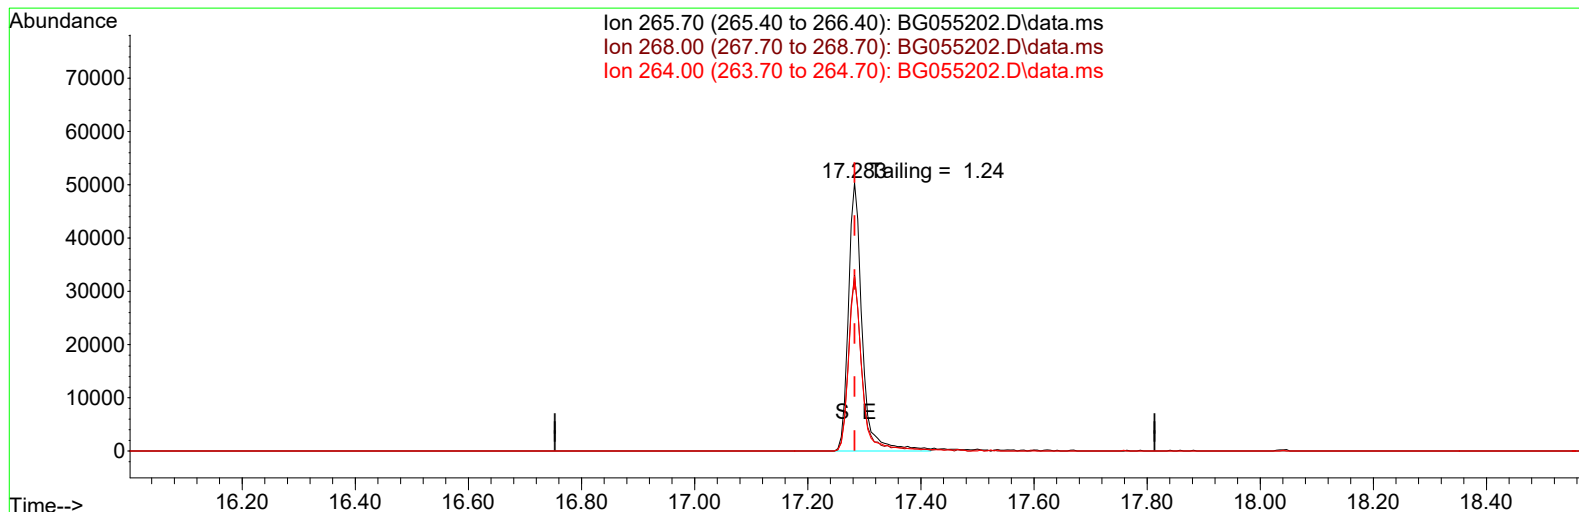

TIC: BG055202.D\data.ms

(70) Pentachlorophenol (C)




17.283min (-0.000) 31193.51 ng

response 86021

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.70	65.39
264.00	63.90	65.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101922\
Data File : BG055202.D
Acq On : 19 Oct 2022 10:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 20 10:07:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 20 09:21:42 2022
Response via : Initial Calibration

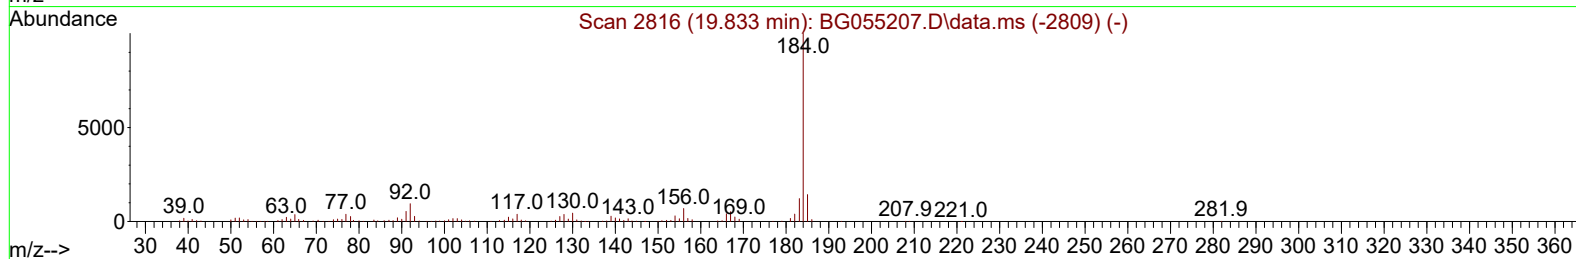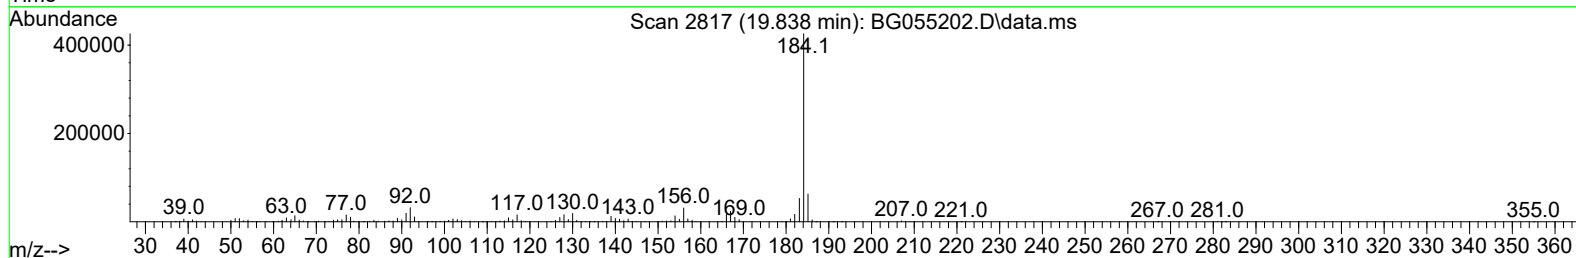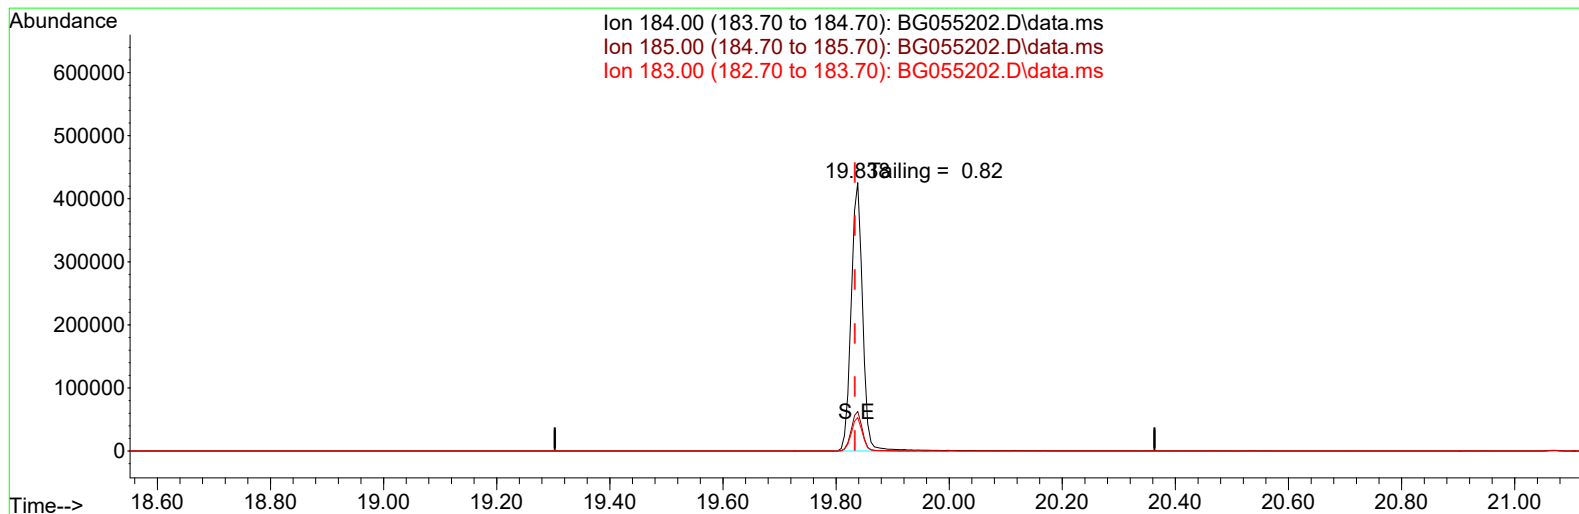

TIC: BG055202.D\data.ms

(77) Benzidine**19.838min (+ 0.005) 0.00 ng****response 602761**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.73
183.00	12.20	12.49
0.00	0.00	0.00