
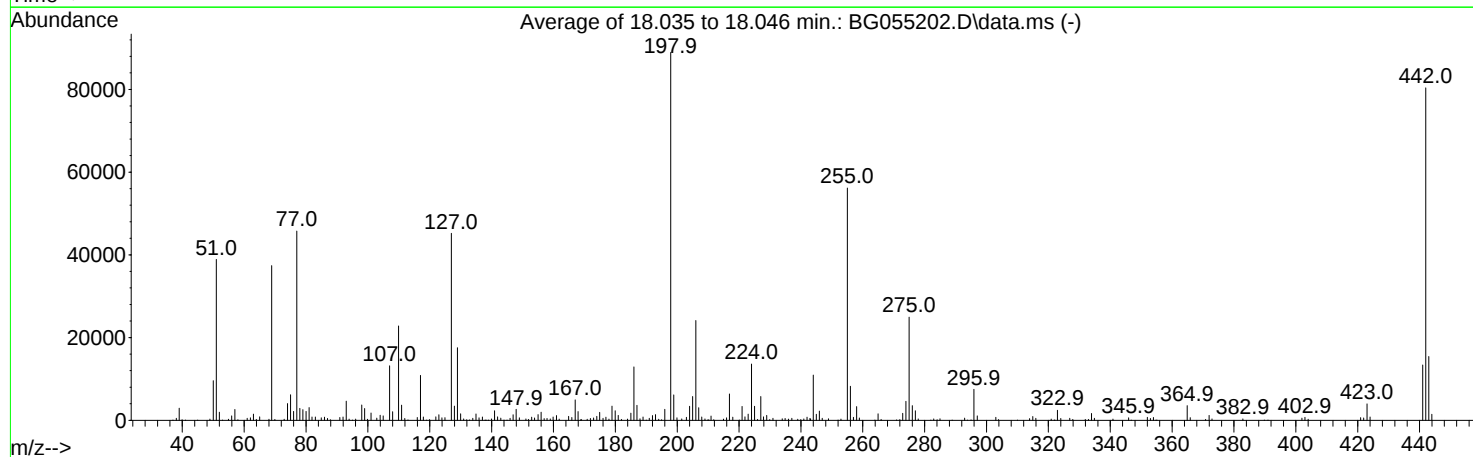


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101922\
 Data File : BG055202.D
 Acq On : 19 Oct 2022 10:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 20 09:21:42 2022

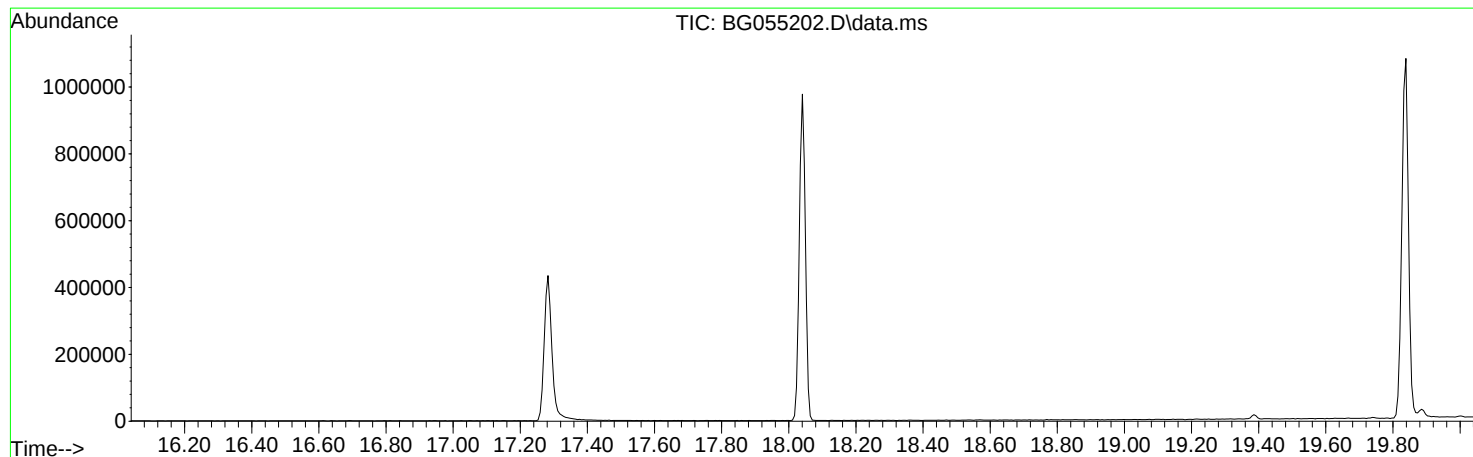




AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.8	38915	PASS
68	69	0.00	2	0.7	250	PASS
69	198	0.00	100	42.0	37379	PASS
70	69	0.00	2	0.6	235	PASS
127	198	10	80	50.8	45205	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	88947	PASS
199	198	5	9	6.9	6141	PASS
275	198	10	60	28.0	24920	PASS
365	198	1	100	4.0	3543	PASS
441	198	0.01	100	15.0	13372	PASS
442	442	50	100	100.0	80387	PASS
443	442	15	24	19.2	15425	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101922\
 Data File : BG055202.D
 Acq On : 19 Oct 2022 10:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Oct 20 10:07:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 20 09:21:42 2022
 Response via : Initial Calibration

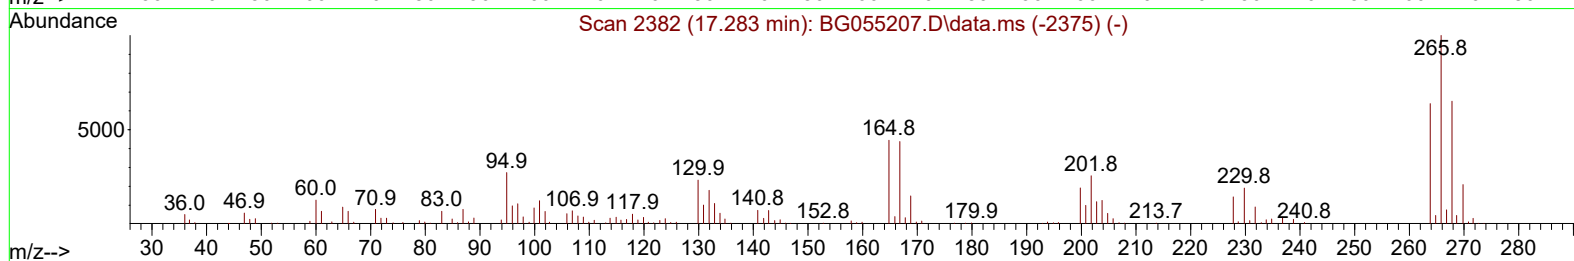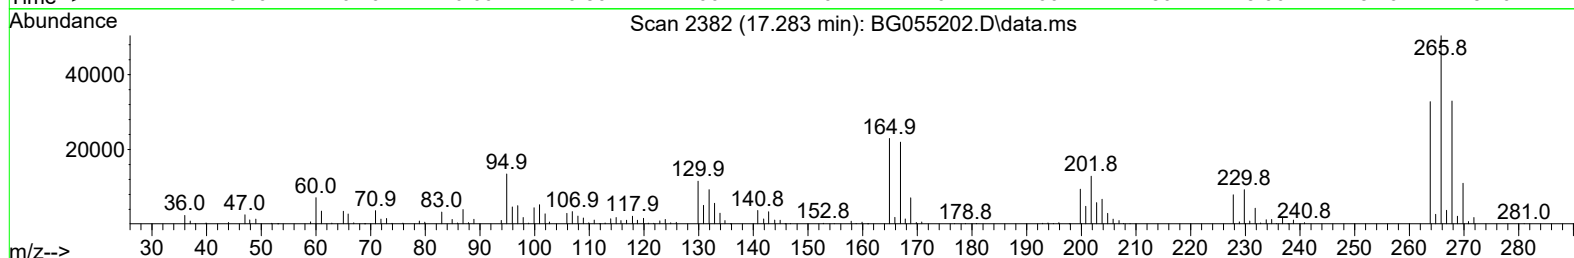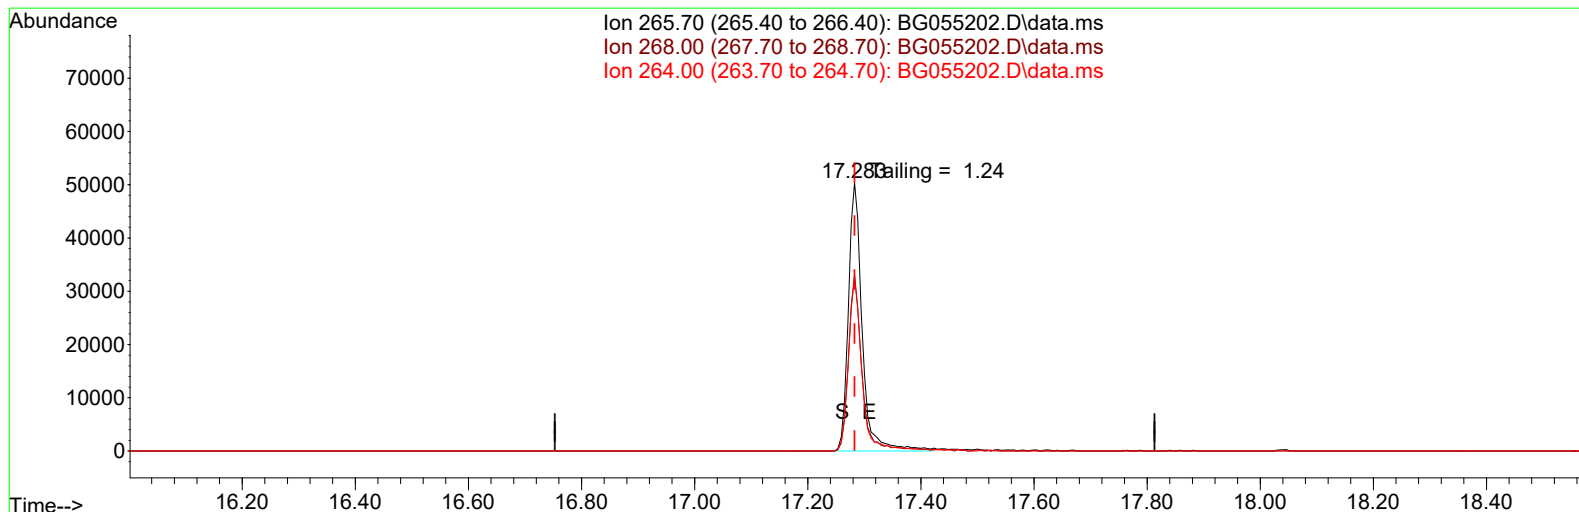

TIC: BG055202.D\data.ms

(70) Pentachlorophenol (C)

17.283min (-0.000) 31193.51 ng




response 86021

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.70	65.39
264.00	63.90	65.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101922\
Data File : BG055202.D
Acq On : 19 Oct 2022 10:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 20 10:07:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 20 09:21:42 2022
Response via : Initial Calibration

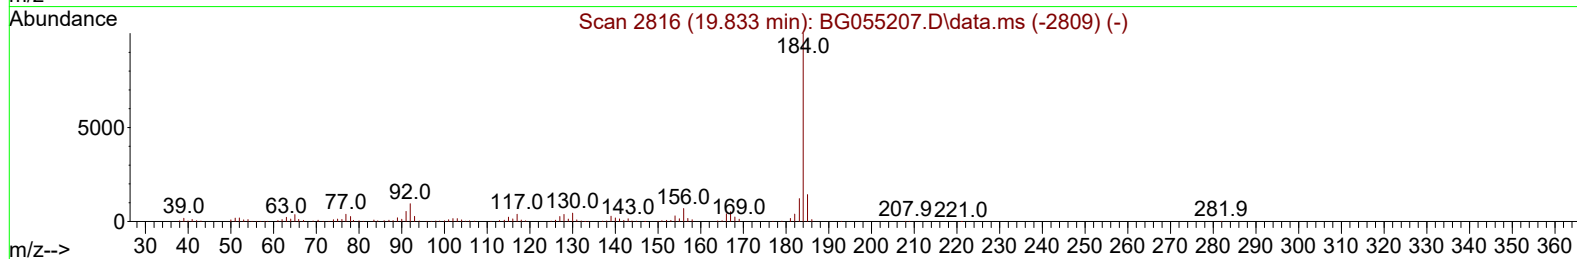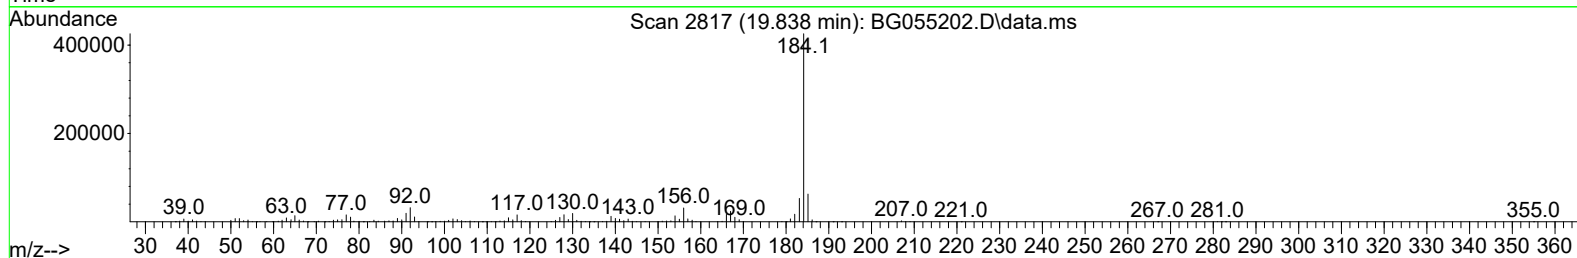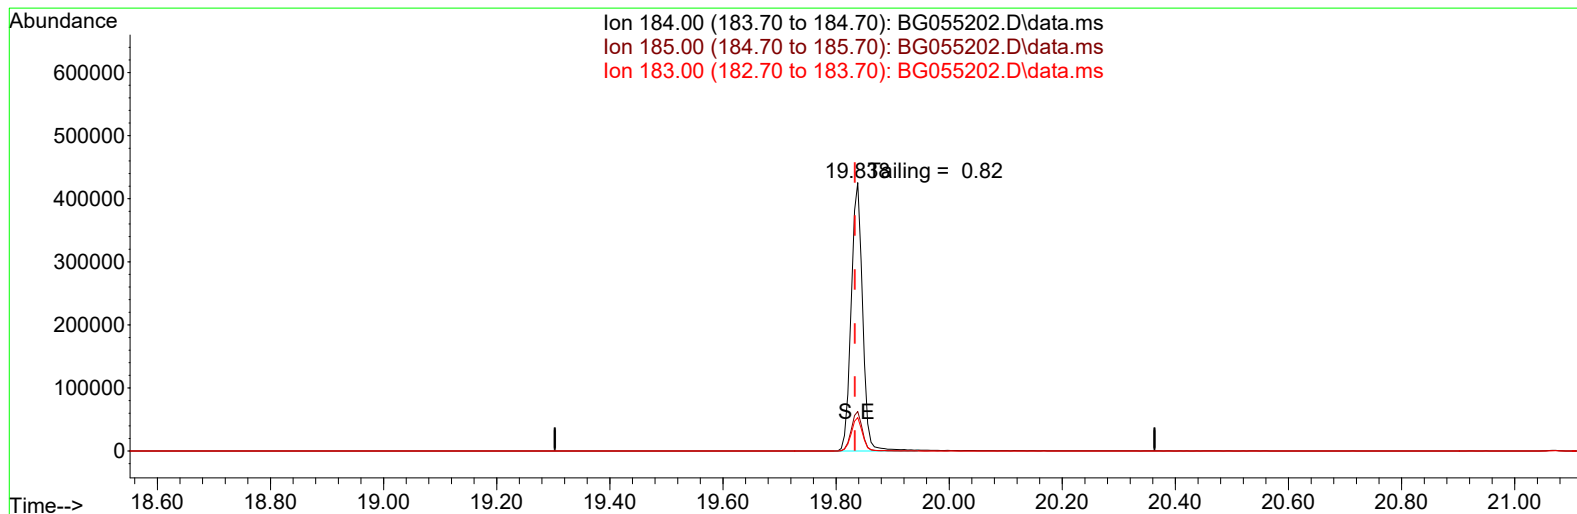

TIC: BG055202.D\data.ms

(77) Benzidine

19.838min (+ 0.005) 0.00 ng

response 602761

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.73
183.00	12.20	12.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/19/2022	BNA_G	<u>BG055202.D</u>
Compound Name	Response	Retention Time
DDT	282356	21.066
DDD	3063	20.673
DDE	0	20.13
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3063	285419	1.07

Instrument :
BNA_G
ClientSampleId :
DFTPP