

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102015\
 Data File : BG019271.D
 Acq On : 20 Oct 2015 23:56
 Operator : UM/NP
 Sample : G4074-20
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9J5

Quant Time: Oct 21 01:26:19 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG101515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 21 01:23:32 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	16089	20.00	ng/ul	0.00
18) Naphthalene-d8	10.79	136	76237	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.62	164	56879	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.37	188	135700	20.00	ng/ul	0.00
78) Chrysene-d12	21.63	240	145360	20.00	ng/ul	0.00
86) Perylene-d12	24.83	264	146642	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.42	96	595	2.06	ng/uL	0.00
5) Phenol-d5	7.17	99	19773	14.08	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.32	67	12636	13.98	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	15161	14.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	16361	13.75	ng/ul	0.00
19) Nitrobenzene-d5	9.15	128	8469	14.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.88	143	10207	16.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.42	165	19312	15.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	20463	12.87	ng/ul	0.00
44) Dimethylphthalate-d6	14.03	166	78390	15.76	ng/ul	0.00
47) Acenaphthylene-d8	14.32	160	90447	16.82	ng/ul	0.00
52) 4-Nitrophenol-d4	14.85	143	12044	13.47	ng/ul	0.00
58) Fluorene-d10	15.62	176	71288	16.77	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	11560	13.81	ng/ul	0.00
71) Anthracene-d10	17.47	188	107754	16.81	ng/ul	0.00
79) Pyrene-d10	19.75	212	123625	18.75	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.61	264	128605	17.36	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.08	163	20174	4.03	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102015\
Data File : BG019271.D
Acq On : 20 Oct 2015 23:56
Operator : UM/NP
Sample : G4074-20
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9J5

Quant Time: Oct 21 01:26:19 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG101515.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 21 01:23:32 2015
Response via : Initial Calibration

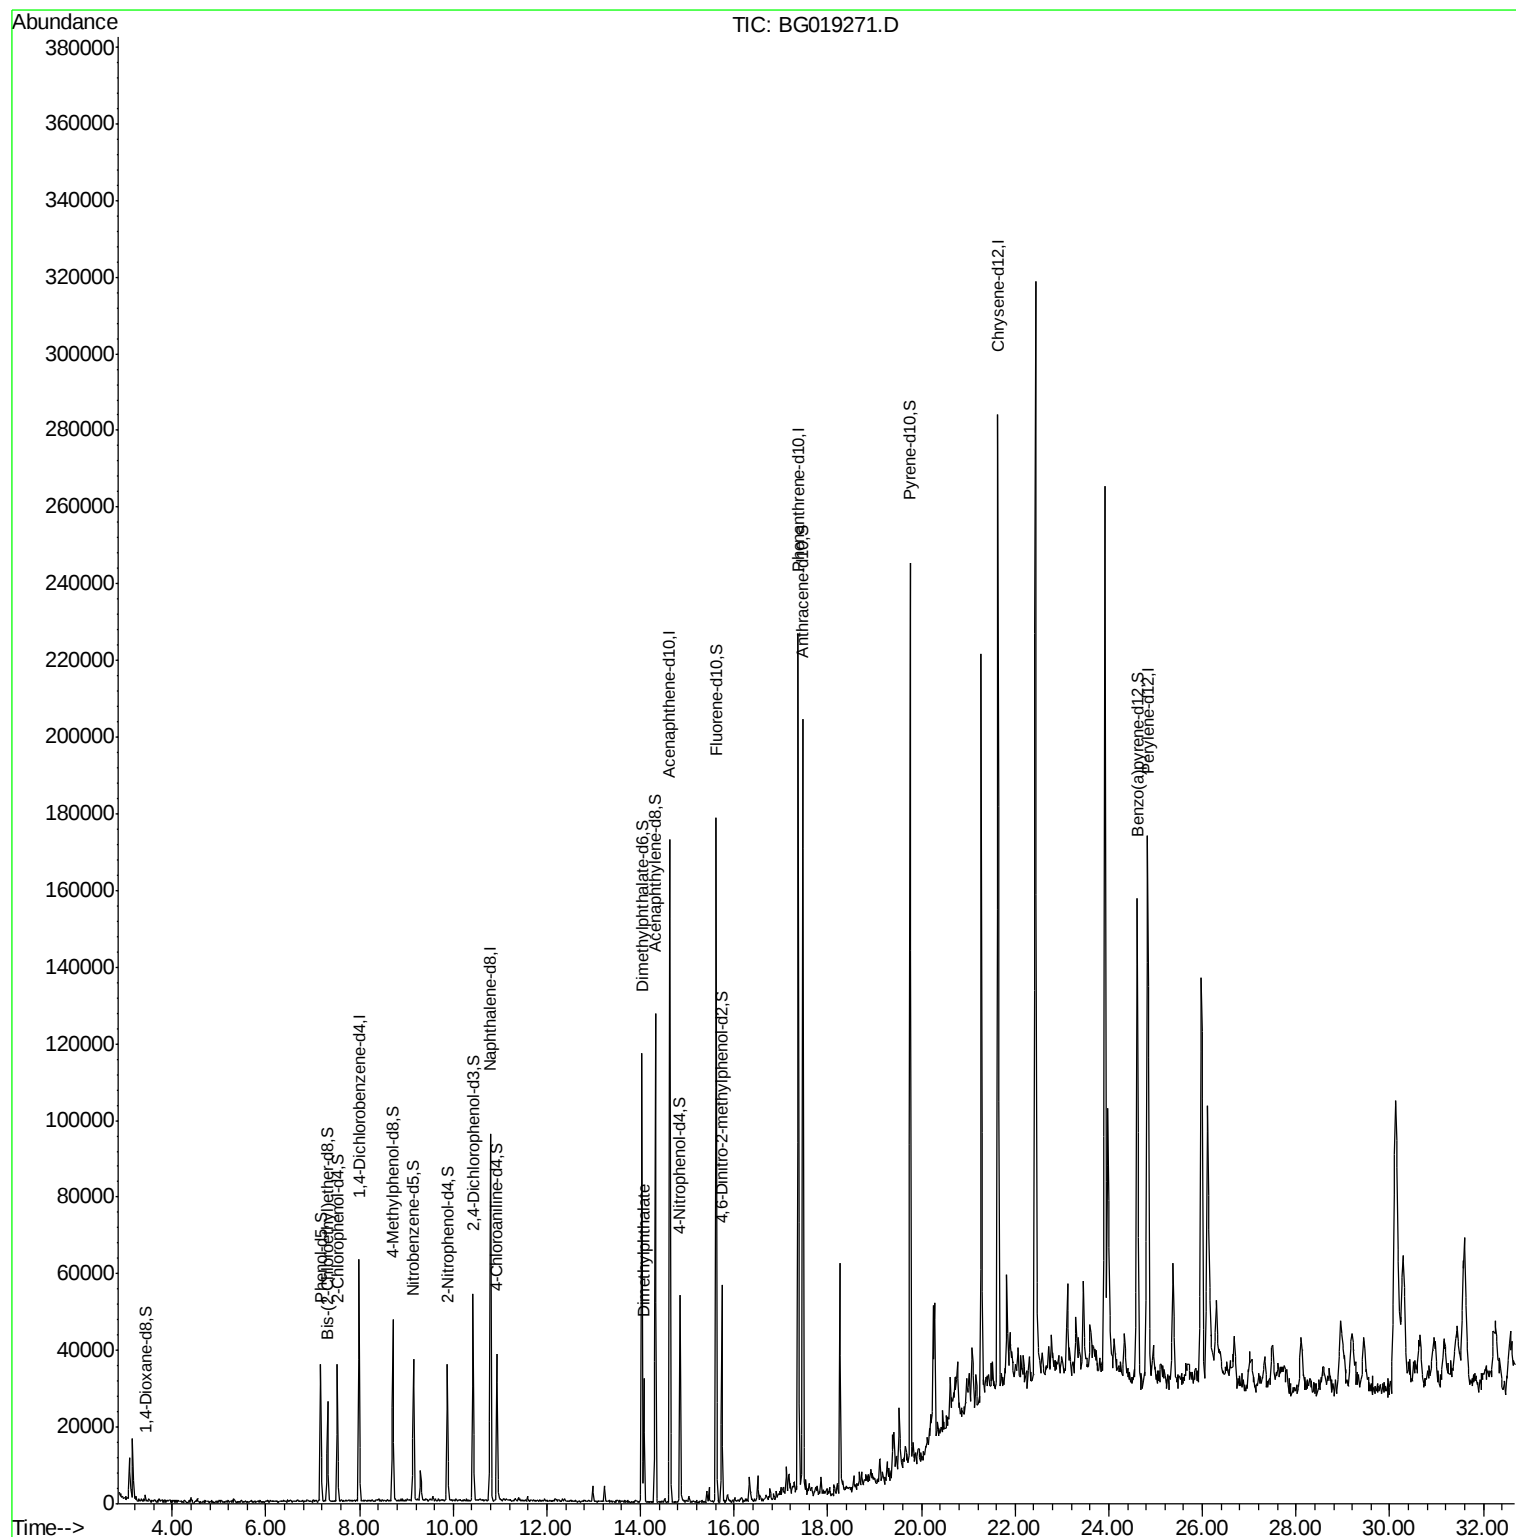

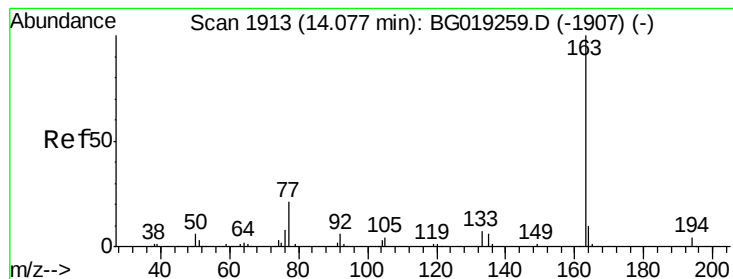

#45

Dimethylphthalate

Concen: 4.03 ng/ul

RT: 14.08 min Scan# 1913

Delta R.T. 0.00 min

Lab File: BG019271.D


Acq: 20 Oct 2015 23:56

Instrument :

BNA_G

ClientSampleId :

JG9J5

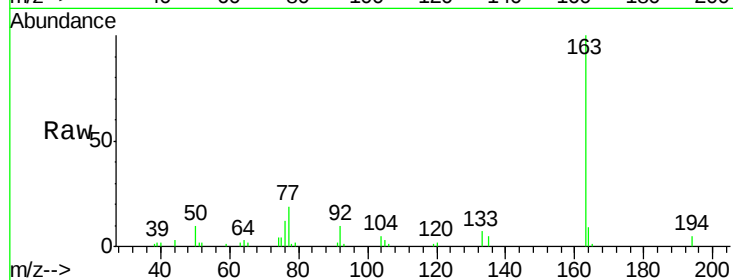

Tgt Ion:	163	Resp:	20174
Ion	Ratio	Lower	Upper
163	100		
194	4.6	3.3	4.9
164	8.9	8.1	12.1

