

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102015\
 Data File : BG019264.D
 Acq On : 20 Oct 2015 19:31
 Operator : UM/NP
 Sample : G4074-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9K2

Quant Time: Oct 21 01:25:36 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG101515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 21 01:23:32 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	15578	20.00	ng/ul	0.00
18) Naphthalene-d8	10.79	136	76443	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.62	164	58598	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.37	188	140249	20.00	ng/ul	0.00
78) Chrysene-d12	21.63	240	145771	20.00	ng/ul	0.00
86) Perylene-d12	24.83	264	146972	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.41	96	537	1.92	ng/uL	-0.01
5) Phenol-d5	7.17	99	13909	10.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.32	67	9770	11.17	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	11248	11.35	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	11459	9.95	ng/ul	0.00
19) Nitrobenzene-d5	9.15	128	6404	10.87	ng/ul	0.00
22) 2-Nitrophenol-d4	9.88	143	7499	12.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.42	165	14230	11.49	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	12144	7.62	ng/ul	0.00
44) Dimethylphthalate-d6	14.02	166	58231	11.36	ng/ul	0.00
47) Acenaphthylene-d8	14.32	160	63588	11.48	ng/ul	0.00
52) 4-Nitrophenol-d4	14.85	143	8335	9.05	ng/ul	0.00
58) Fluorene-d10	15.62	176	51893	11.85	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	8703	10.06	ng/ul	0.00
71) Anthracene-d10	17.47	188	79661	12.02	ng/ul	0.00
79) Pyrene-d10	19.75	212	82170	12.43	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.61	264	84904	11.44	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.08	163	12405	2.40	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102015\
Data File : BG019264.D
Acq On : 20 Oct 2015 19:31
Operator : UM/NP
Sample : G4074-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9K2

Quant Time: Oct 21 01:25:36 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG101515.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 21 01:23:32 2015
Response via : Initial Calibration

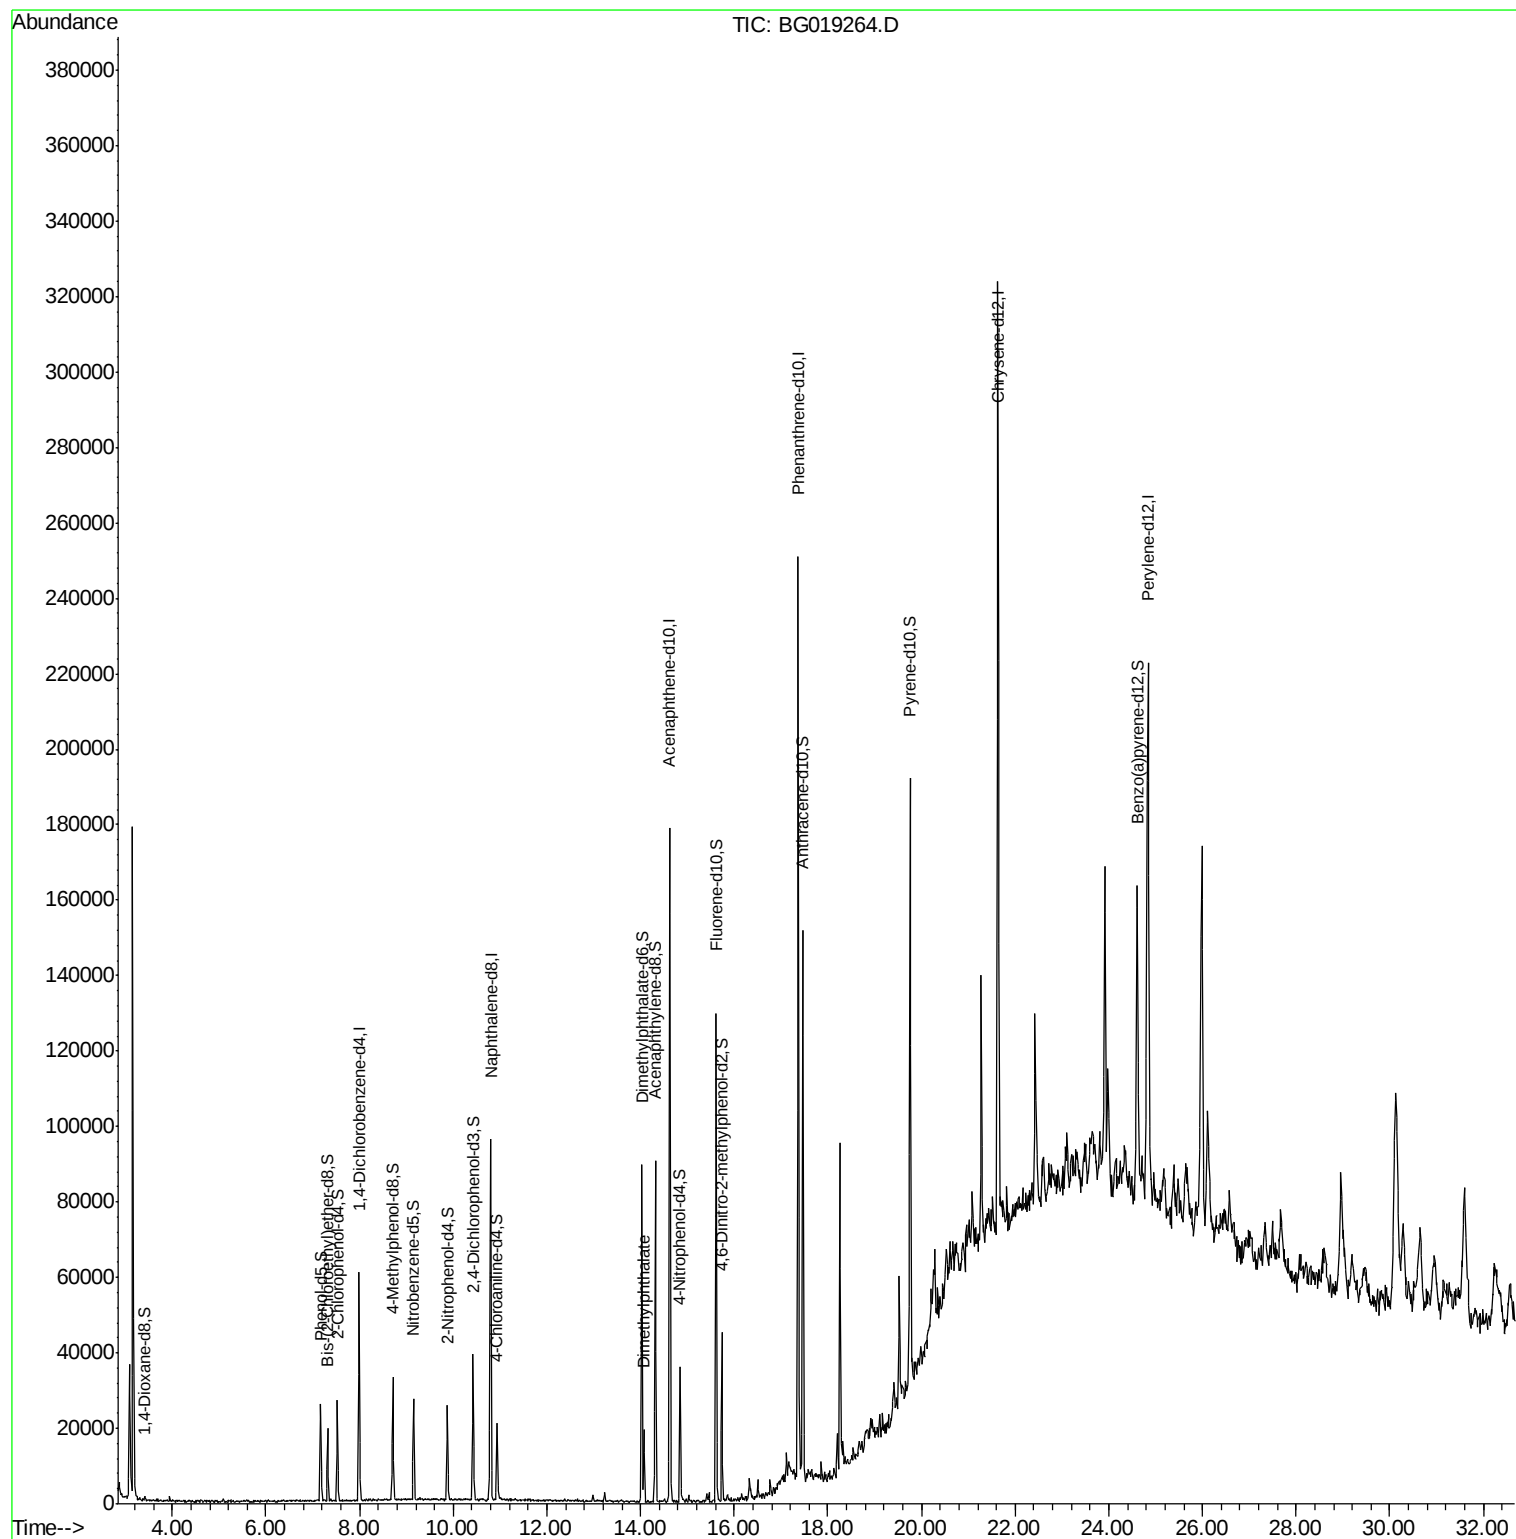

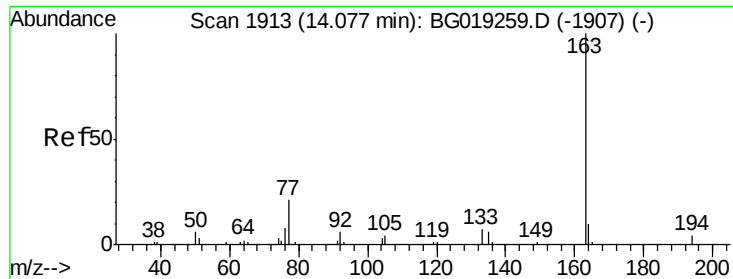

#45

Dimethylphthalate

Concen: 2.40 ng/ul

RT: 14.08 min Scan# 1913

Delta R.T. 0.00 min

Lab File: BG019264.D


Acq: 20 Oct 2015 19:31

Instrument :

BNA_G

ClientSampleId :

JG9K2

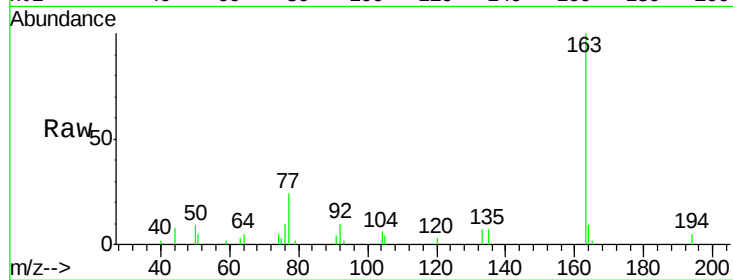


Tgt Ion:163 Resp: 12405

Ion Ratio Lower Upper

163 100

194 4.9 3.3 4.9

164 9.3 8.1 12.1

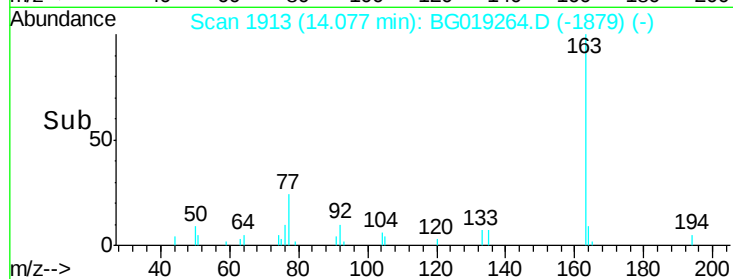

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

