

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102015\
 Data File : BG019265.D
 Acq On : 20 Oct 2015 20:08
 Operator : UM/NP
 Sample : G4074-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9K3

Quant Time: Oct 21 01:25:42 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG101515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 21 01:23:32 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	15050	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	70721	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.62	164	54744	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.37	188	134786	20.00	ng/ul	0.00
78) Chrysene-d12	21.63	240	140477	20.00	ng/ul	0.00
86) Perylene-d12	24.83	264	143331	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.42	96	346	1.28	ng/uL	0.00
5) Phenol-d5	7.17	99	13605	10.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.31	67	8770	10.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	11124	11.62	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	11290	10.15	ng/ul	0.00
19) Nitrobenzene-d5	9.15	128	5739	10.53	ng/ul	0.00
22) 2-Nitrophenol-d4	9.88	143	6825	11.80	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	14741	12.87	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	13163	8.92	ng/ul	0.00
44) Dimethylphthalate-d6	14.03	166	59834	12.50	ng/ul	0.00
47) Acenaphthylene-d8	14.32	160	65869	12.73	ng/ul	0.00
52) 4-Nitrophenol-d4	14.84	143	9189	10.68	ng/ul	0.00
58) Fluorene-d10	15.62	176	53894	13.17	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	9988	12.01	ng/ul	0.00
71) Anthracene-d10	17.47	188	86475	13.58	ng/ul	0.00
79) Pyrene-d10	19.75	212	93931	14.74	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.61	264	94259	13.02	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.08	163	18369	3.81	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102015\
Data File : BG019265.D
Acq On : 20 Oct 2015 20:08
Operator : UM/NP
Sample : G4074-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9K3

Quant Time: Oct 21 01:25:42 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG101515.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 21 01:23:32 2015
Response via : Initial Calibration

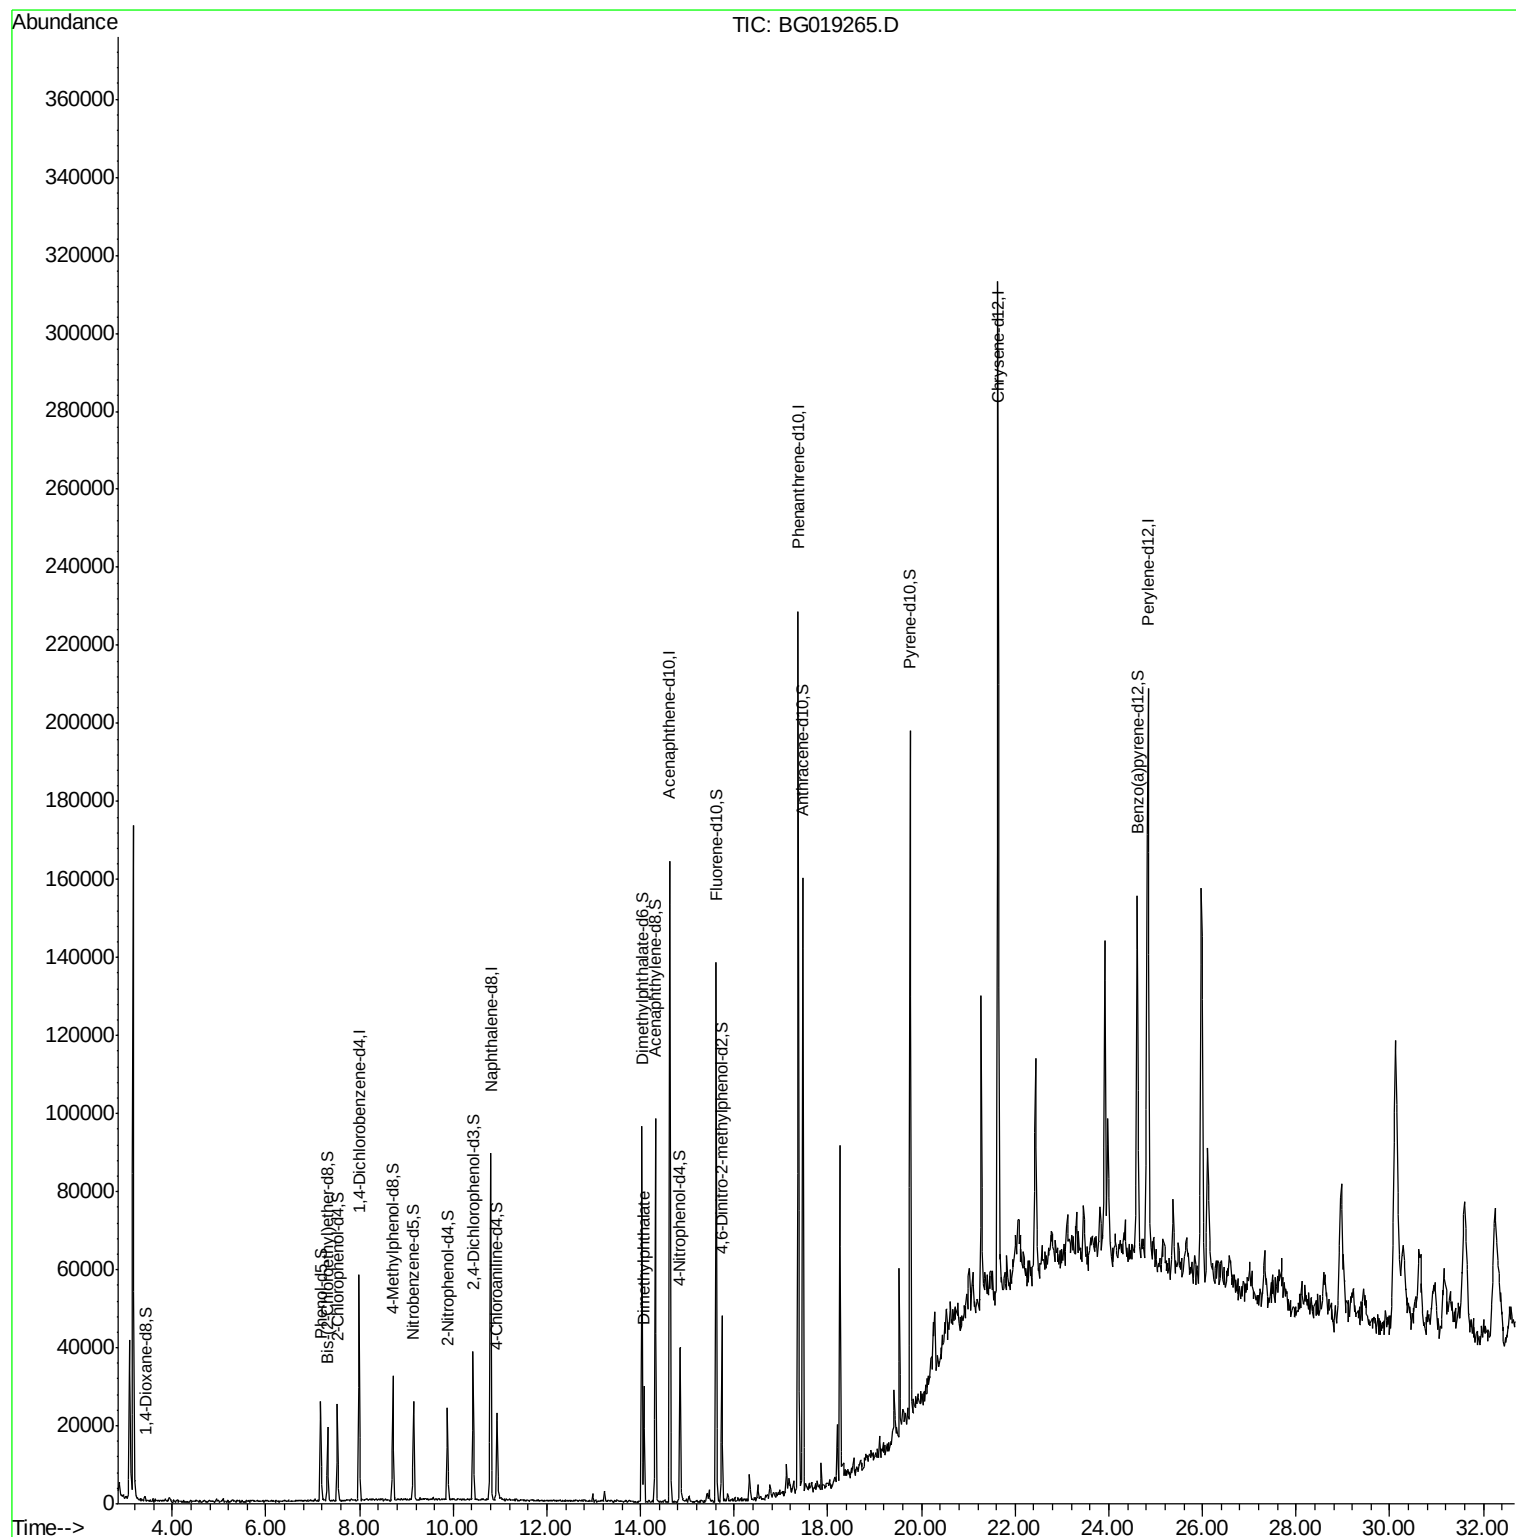

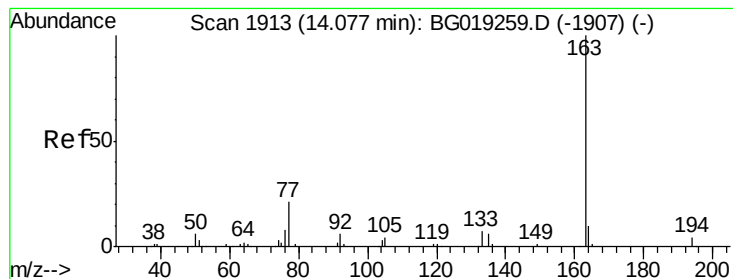

#45

Dimethylphthalate

Concen: 3.81 ng/ul

RT: 14.08 min Scan# 1913

Delta R.T. -0.00 min

Lab File: BG019265.D


Acq: 20 Oct 2015 20:08

Instrument :

BNA_G

ClientSampleId :

JG9K3

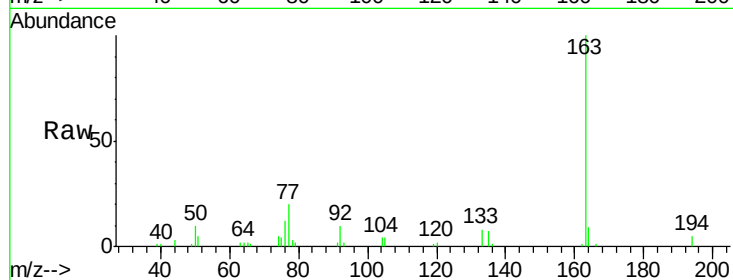

Tgt Ion:	163	Resp:	18369
Ion	Ratio	Lower	Upper
163	100		
194	5.1	3.3	4.9#
164	8.6	8.1	12.1

