

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102015\
 Data File : BG019269.D
 Acq On : 20 Oct 2015 22:40
 Operator : UM/NP
 Sample : G4074-18
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9H7

Quant Time: Oct 21 01:26:07 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG101515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 21 01:23:32 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	16924	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	80489	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.62	164	58017	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.37	188	142090	20.00	ng/ul	0.00
78) Chrysene-d12	21.63	240	149643	20.00	ng/ul	0.00
86) Perylene-d12	24.84	264	152432	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.42	96	658	2.17	ng/uL	0.00
5) Phenol-d5	7.17	99	16984	11.50	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.31	67	11438	12.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	13798	12.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	13933	11.13	ng/ul	0.00
19) Nitrobenzene-d5	9.15	128	7373	11.89	ng/ul	0.00
22) 2-Nitrophenol-d4	9.87	143	9081	13.80	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.42	165	16420	12.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	15748	9.38	ng/ul	0.00
44) Dimethylphthalate-d6	14.03	166	66283	13.06	ng/ul	0.00
47) Acenaphthylene-d8	14.32	160	74312	13.55	ng/ul	0.00
52) 4-Nitrophenol-d4	14.84	143	8559	9.38	ng/ul	0.00
58) Fluorene-d10	15.62	176	58784	13.55	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	9055	10.33	ng/ul	0.00
71) Anthracene-d10	17.47	188	87005	12.96	ng/ul	0.00
79) Pyrene-d10	19.75	212	93704	13.81	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.61	264	98337	12.77	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.08	163	22019	4.31	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102015\
Data File : BG019269.D
Acq On : 20 Oct 2015 22:40
Operator : UM/NP
Sample : G4074-18
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9H7

Quant Time: Oct 21 01:26:07 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG101515.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 21 01:23:32 2015
Response via : Initial Calibration

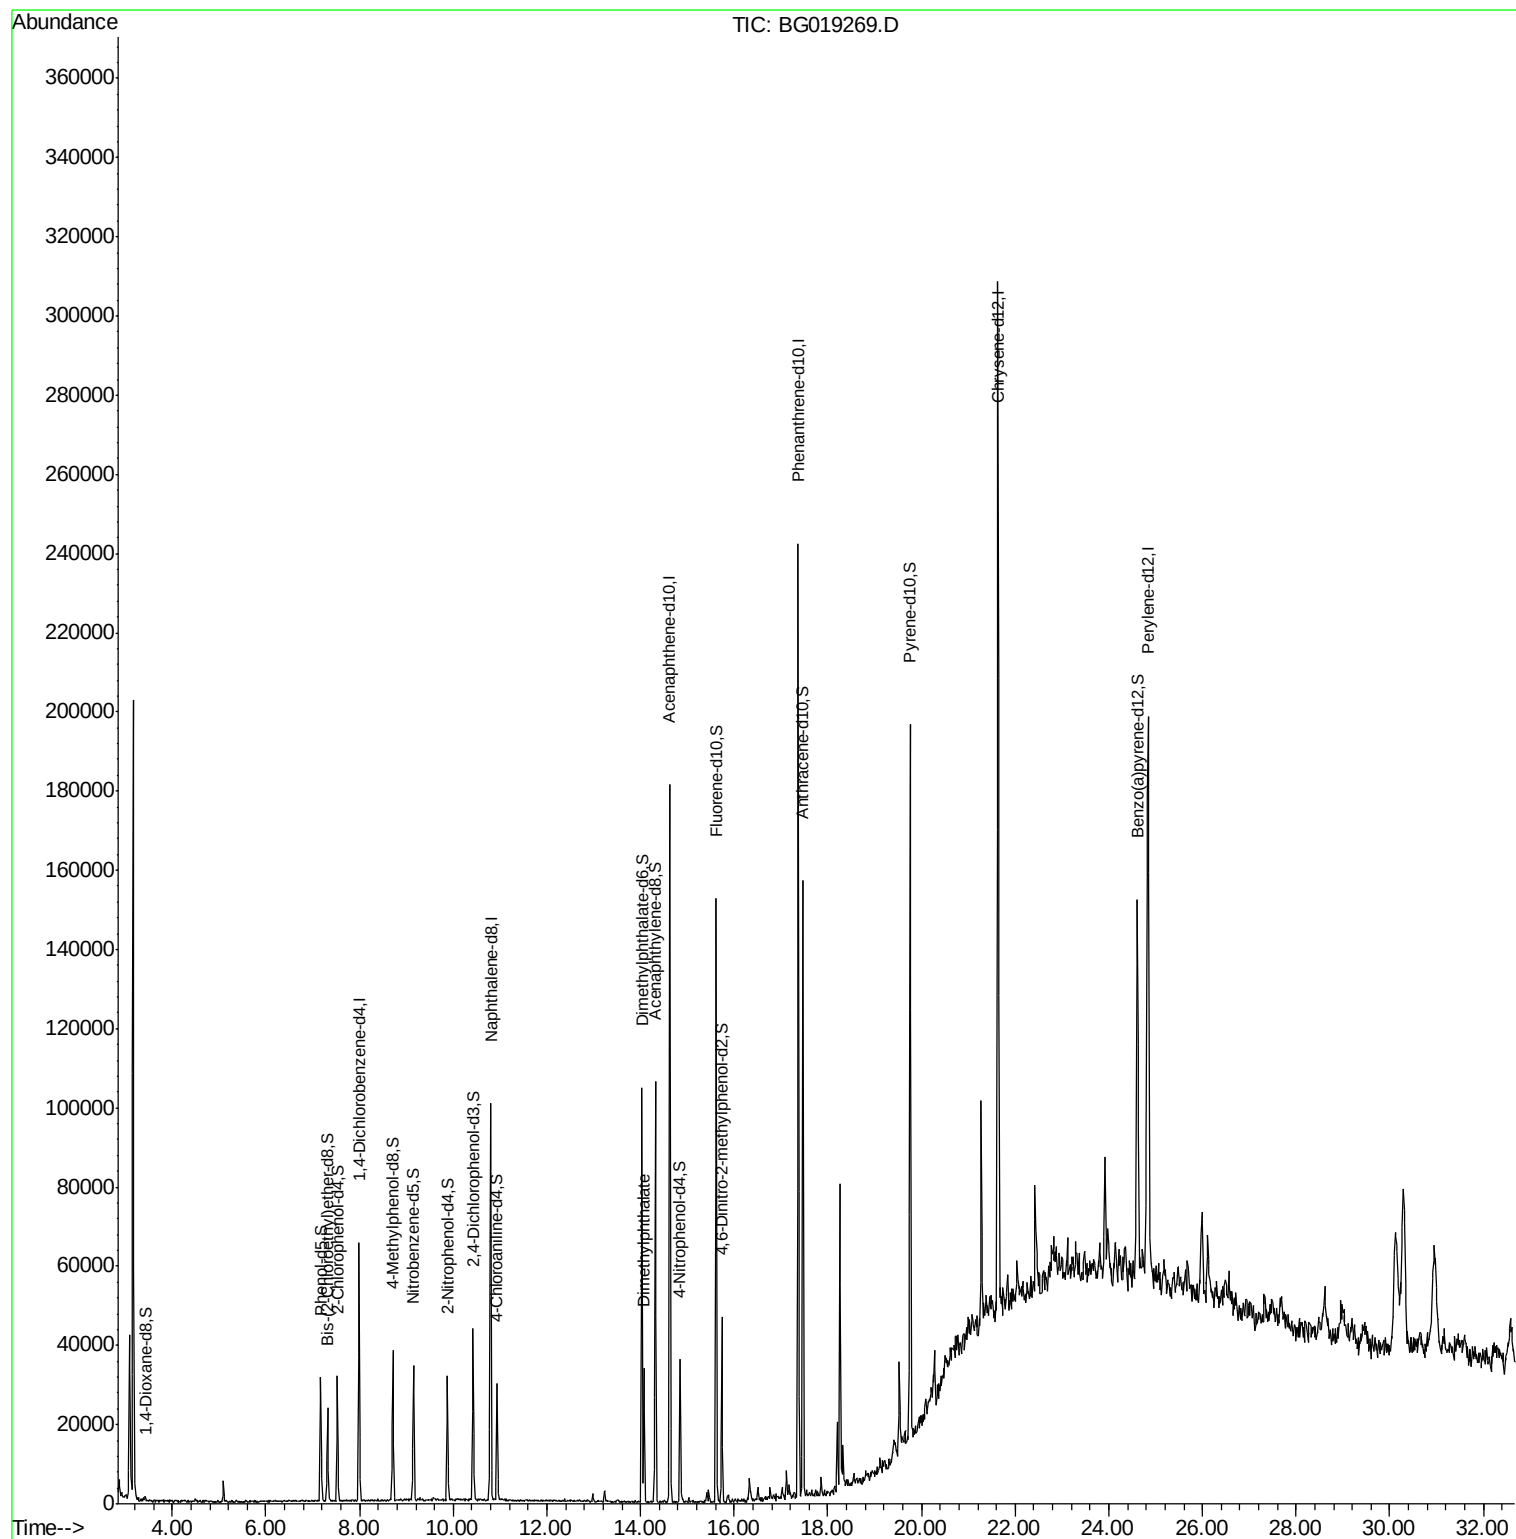

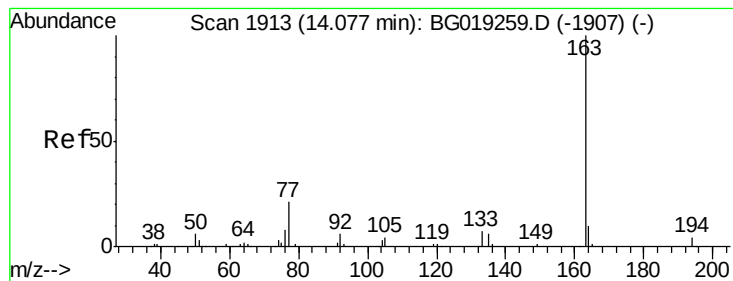

#45

Dimethylphthalate

Concen: 4.31 ng/ul

RT: 14.08 min Scan# 1913

Delta R.T. 0.00 min

Lab File: BG019269.D


Acq: 20 Oct 2015 22:40

Instrument :

BNA_G

ClientSampleId :

JG9H7

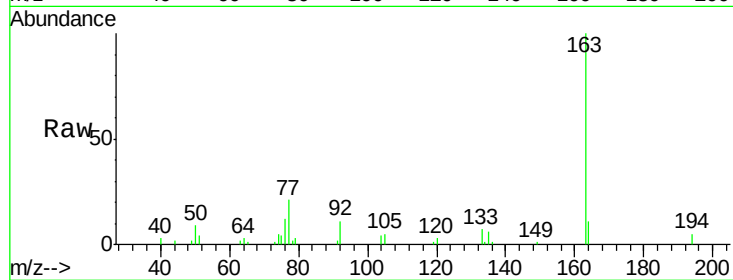

Tgt Ion:163 Resp: 22019

Ion Ratio Lower Upper

163 100

194 4.7 3.3 4.9

164 10.5 8.1 12.1

