


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102015\
 Data File : BG019258.D
 Acq On : 20 Oct 2015 15:34
 Operator : UM/NP
 Sample : DFTPP05
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP05

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG101515.M
 Title : SVOA CALIBRATION
 Last Update : Wed Oct 21 11:24:25 2015

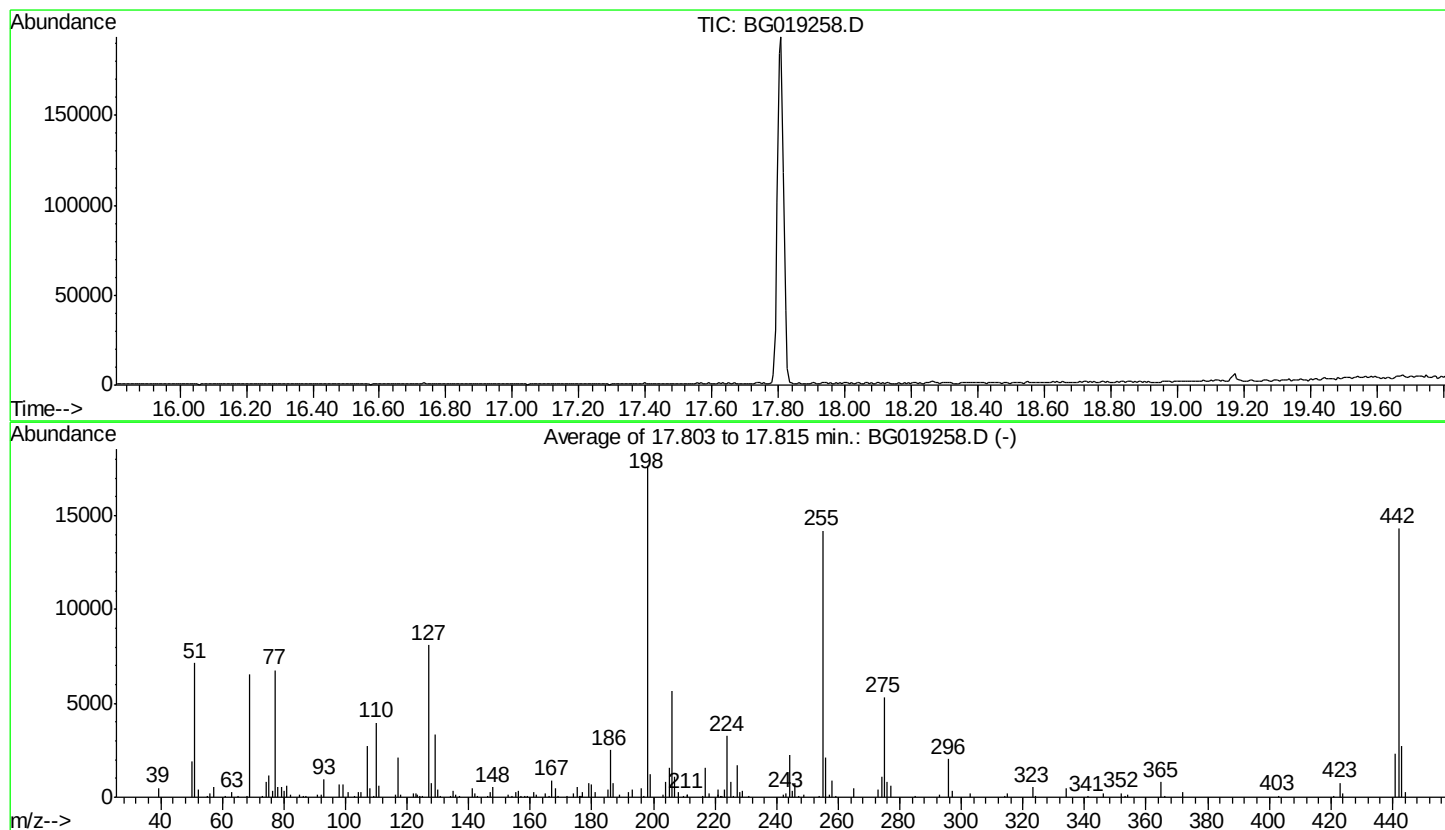

AutoFind: Scans 2547, 2548, 2549; Background Corrected with Scan 2542

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	7125	PASS
68	69	0.00	2	0.8	53	PASS
69	198	0.00	100	37.2	6564	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.9	8101	PASS
197	198	0.00	2	0.5	89	PASS
198	198	100	100	100.0	17650	PASS
199	198	5	9	7.2	1262	PASS
275	198	10	60	30.0	5298	PASS
365	198	1	100	4.5	803	PASS
441	442	0.01	24	16.1	2294	PASS
442	198	50	100	81.0	14289	PASS
443	442	15	24	19.0	2721	PASS

m/z	Abundance
39.10	623.0
40.00	288.0
44.10	524.0
50.10	2261.0
51.10	9360.0
52.10	508.0
56.00	377.0
57.10	709.0
61.00	206.0
63.00	292.0
68.00	159.0
69.00	8619.0
73.10	174.0
74.10	1060.0
75.10	1531.0
76.10	536.0
77.10	8437.0
78.10	596.0
79.00	568.0
80.00	552.0
81.00	773.0
82.10	191.0
85.00	254.0
87.10	190.0
91.00	242.0
92.00	254.0
93.10	1076.0
98.00	839.0
99.00	819.0
101.00	391.0
103.90	326.0
105.00	296.0
107.00	3139.0
108.00	628.0
110.00	4648.0
111.00	581.0
116.00	310.0
117.10	2336.0
118.00	184.0
122.10	243.0
122.90	359.0
124.00	172.0
125.10	173.0
127.10	9914.0
128.00	1018.0
129.00	4058.0
130.00	503.0
135.10	392.0
141.00	525.0
142.00	213.0
147.10	237.0
148.00	693.0
153.00	156.0
155.10	357.0
156.00	373.0
161.00	303.0
162.20	159.0
164.90	241.0
166.00	183.0
167.00	903.0
168.10	632.0
171.90	168.0
174.10	354.0
175.10	645.0
175.90	161.0
177.00	278.0
179.00	815.0
180.00	799.0
180.90	211.0
185.10	558.0
186.00	2542.0
187.00	876.0
189.00	344.0
192.00	256.0
193.00	341.0
196.10	440.0
198.00	18976.0
199.00	1438.0
202.90	220.0
204.00	925.0
205.10	1885.0
206.00	6107.0
207.00	1245.0
208.00	282.0
210.90	283.0
217.00	1449.0
218.00	238.0
220.90	453.0
221.70	312.0
222.90	440.0
224.00	3828.0

Instrument :
BNA_G
ClientSampleId :
DFTPP05

225.00	941.0
227.00	1864.0
228.00	234.0
229.00	332.0
242.10	187.0
243.10	280.0
244.10	2387.0
244.90	389.0
246.00	790.0
249.00	150.0
253.90	200.0
255.00	14916.0
256.00	2594.0
257.00	196.0
258.00	949.0
265.00	495.0
273.00	484.0
274.10	1114.0
275.00	5345.0
276.00	1120.0
277.00	737.0
293.10	207.0
296.00	2069.0
297.00	402.0
303.00	191.0
315.00	217.0
323.10	565.0
334.00	511.0
345.90	163.0
352.00	244.0
354.00	265.0
364.90	608.0
366.10	190.0
372.10	185.0
423.00	730.0
423.90	233.0
441.00	1990.0
442.00	13439.0
443.00	2474.0
444.10	284.0

Instrument :
BNA_G
ClientSampleId :
DFTPP05

m/z	Abundance
39.10	526.0
44.10	487.0
50.10	2348.0
51.10	7705.0
52.10	449.0
55.00	215.0
56.00	241.0
57.10	522.0
63.10	291.0
65.00	277.0
69.00	7224.0
74.10	835.0
75.00	1171.0
76.10	357.0
77.10	7863.0
78.10	790.0
79.10	699.0
80.00	318.0
81.00	795.0
82.10	202.0
85.10	182.0
86.20	211.0
91.00	164.0
92.10	221.0
93.00	1110.0
98.00	712.0
99.00	780.0
101.00	340.0
103.00	164.0
104.00	309.0
105.10	289.0
107.00	2972.0
108.00	422.0
109.20	181.0
110.10	4423.0
111.00	707.0
116.10	153.0
117.00	2484.0
118.00	185.0
121.90	189.0
123.10	326.0
127.00	8951.0
128.00	957.0
129.00	3837.0
130.00	409.0
130.90	154.0
134.00	223.0
135.00	375.0
135.90	216.0
137.10	206.0
141.10	622.0
142.00	357.0
143.00	248.0
146.00	175.0
147.00	311.0
148.00	513.0
154.10	164.0
155.10	409.0
156.00	492.0
157.10	159.0
158.10	202.0
159.10	165.0
160.90	269.0
162.00	178.0
165.00	228.0
167.00	1050.0
168.00	507.0
169.10	155.0
174.00	189.0
175.00	661.0
176.10	157.0
176.90	255.0
179.00	1008.0
180.00	791.0
181.00	271.0
185.10	470.0
186.10	3147.0
187.00	984.0
192.00	263.0
193.00	498.0
196.00	484.0
196.90	267.0
198.00	20664.0
199.00	1467.0
203.00	173.0
204.00	951.0
205.00	1612.0
206.00	6740.0
207.00	1096.0
208.00	370.0
211.10	322.0

Instrument :
BNA_G
ClientSampleId :
DFTPP05

217.00	2156.0
218.00	310.0
221.10	871.0
222.00	251.0
223.00	466.0
224.00	3630.0
225.00	917.0
225.90	168.0
227.00	2019.0
227.90	344.0
229.00	336.0
230.90	233.0
242.00	152.0
243.00	198.0
244.00	2687.0
245.00	358.0
246.00	842.0
247.00	198.0
249.00	169.0
255.00	17312.0
256.00	2275.0
257.00	201.0
258.00	984.0
265.00	540.0
272.90	507.0
274.00	1356.0
275.00	6379.0
276.00	805.0
277.00	728.0
285.10	169.0
292.90	155.0
295.90	2154.0
297.00	316.0
303.00	277.0
314.00	234.0
315.00	269.0
323.00	673.0
324.00	187.0
334.00	462.0
341.10	187.0
345.90	225.0
352.10	160.0
353.00	201.0
354.00	242.0
364.90	1072.0
372.00	398.0
403.00	240.0
421.10	158.0
423.00	773.0
423.90	229.0
441.00	2979.0
442.00	16752.0
443.00	3208.0
444.00	303.0

Instrument :
BNA_G
ClientSampleId :
DFTPP05

m/z	Abundance
39.10	295.0
44.10	612.0
50.10	1178.0
51.10	4311.0
52.10	298.0
57.00	314.0
63.00	153.0
69.00	3849.0
74.10	508.0
75.10	785.0
76.10	207.0
77.10	4001.0
78.10	291.0
79.00	411.0
80.10	217.0
81.00	185.0
93.00	673.0
98.00	507.0
99.00	395.0
101.00	187.0
103.90	160.0
104.90	220.0
107.00	2072.0
108.00	476.0
110.00	2793.0
111.00	494.0
117.00	1564.0
122.00	160.0
122.90	281.0
127.00	5440.0
128.10	381.0
129.00	2188.0
130.00	256.0
135.00	244.0
135.90	174.0
140.90	337.0
146.90	192.0
148.00	406.0
152.90	193.0
156.00	256.0
161.00	172.0
164.90	187.0
167.10	633.0
168.00	326.0
174.00	165.0
175.10	306.0
176.40	185.0
177.10	236.0
178.90	405.0
180.00	447.0
181.00	375.0
185.00	278.0
186.10	1843.0
187.00	486.0
192.00	243.0
193.00	369.0
196.00	558.0
198.00	13311.0
199.00	881.0
204.00	568.0
205.00	1154.0
206.10	4043.0
206.90	873.0
208.10	169.0
209.90	196.0
210.90	176.0
216.10	191.0
217.00	1161.0
218.00	168.0
221.00	364.0
222.90	369.0
224.00	2340.0
225.00	547.0
227.00	1307.0
227.90	172.0
229.10	319.0
242.00	164.0
243.20	170.0
244.10	1586.0
245.00	226.0
246.00	561.0
255.00	10306.0
256.00	1483.0
258.00	809.0
259.00	169.0
265.10	311.0
272.90	324.0
274.00	902.0
275.00	4172.0
275.90	582.0
277.10	319.0

Instrument :
BNA_G
ClientSampleId :
DFTPP05

296.00	1833.0
297.00	297.0
303.10	182.0
315.00	173.0
323.10	385.0
333.90	436.0
346.00	181.0
352.10	245.0
365.00	730.0
372.00	183.0
423.00	775.0
424.00	160.0
441.00	1913.0
442.00	12678.0
443.00	2483.0
444.10	240.0

Instrument :
BNA_G
ClientSampleId :
DFTPP05

Scan 2542 (17.773 min): BG019258.D
DFTPP05

m/z	Abundance
40.00	151.0
44.10	591.0
207.20	320.0

Instrument :
BNA_G
ClientSampleId :
DFTPP05