


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102016\
Data File : BG024456.D
Acq On : 20 Oct 2016 10:45
Operator : UM/SJ
Sample : DFTPP10
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102016-MA.M
Title : SVOA CALIBRATION
Last Update : Fri Oct 21 18:36:46 2016

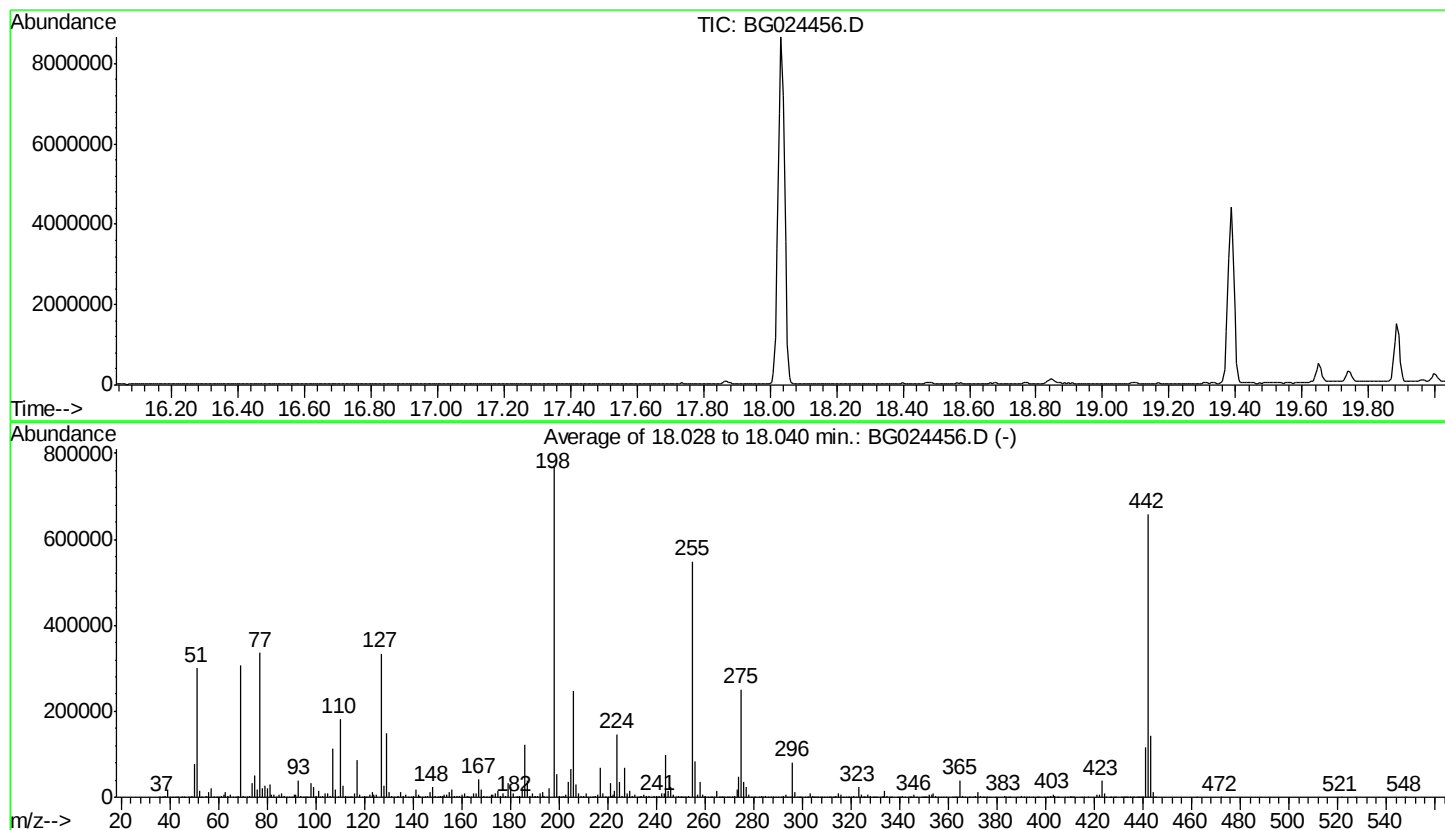

AutoFind: Scans 2585, 2586, 2587; Background Corrected with Scan 2579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	301744	PASS
68	69	0.00	2	1.3	4097	PASS
69	198	0.00	100	39.9	307586	PASS
70	69	0.00	2	0.6	1703	PASS
127	198	10	80	43.4	335125	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	771712	PASS
199	198	5	9	6.9	53525	PASS
275	198	10	60	32.5	251072	PASS
365	198	1	100	5.1	39330	PASS
441	443	0.01	100	81.5	116322	PASS
442	198	50	100	85.4	659178	PASS
443	442	15	24	21.7	142752	PASS